

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017768.D
 Acq On : 31 Jul 2020 12:18
 Operator : SY/MD
 Sample : VV0731WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK31

Quant Time: Aug 01 04:56:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	169000	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	162403	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	83335	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34677	4.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.00%
7) Chloroethane-d5	1.58	69	29421	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.20%
11) 1,1-Dichloroethene-d2	2.12	63	56857	3.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.80%
20) 2-Butanone-d5	3.95	46	83403	43.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.40%
24) Chloroform-d	4.37	84	86717	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	5.06	65	49789	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.07	84	146906	4.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.00%
36) 1,2-Dichloropropane-d6	6.09	67	39956	4.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.20%
41) Toluene-d8	7.34	98	132050	3.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.00%
45) trans-1,3-Dichloropropene-	7.64	79	17789	3.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.80%
48) 2-Hexanone-d5	8.11	63	53166	38.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.08%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	27298	3.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	55496	4.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.00%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	4187	0.413 ug/L	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017768.D
Acq On : 31 Jul 2020 12:18
Operator : SY/MD
Sample : VV0731WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK31

Quant Time: Aug 01 04:56:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 01 04:42:38 2020
Response via : Initial Calibration

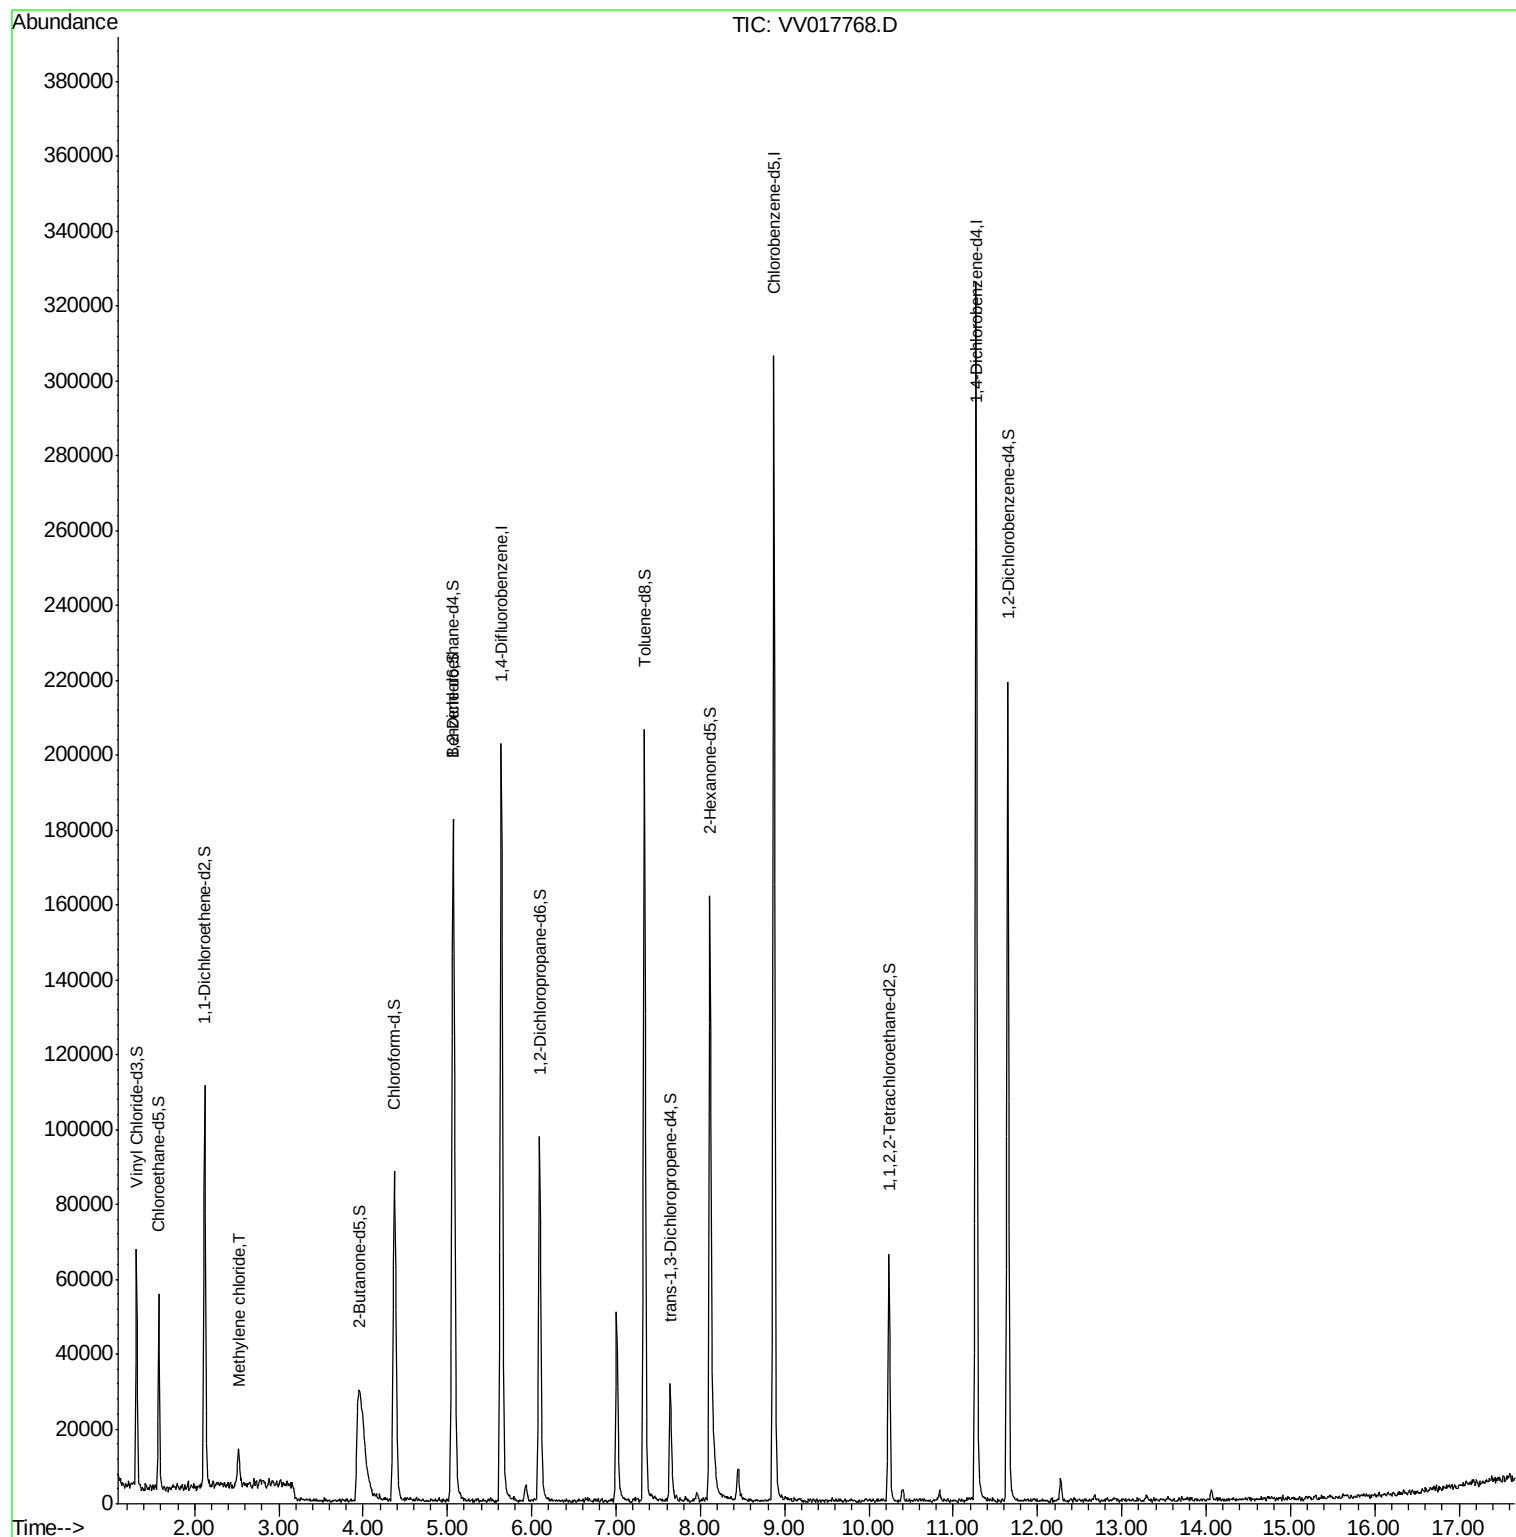

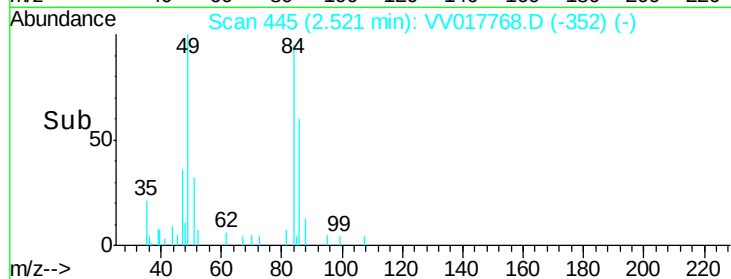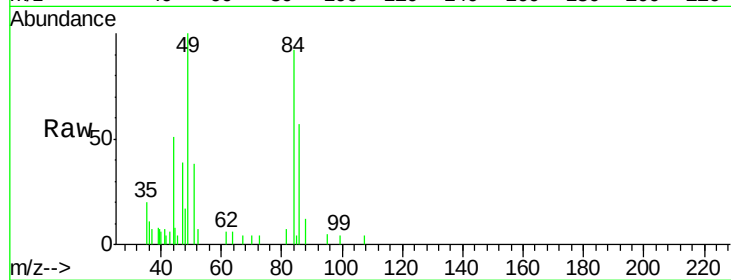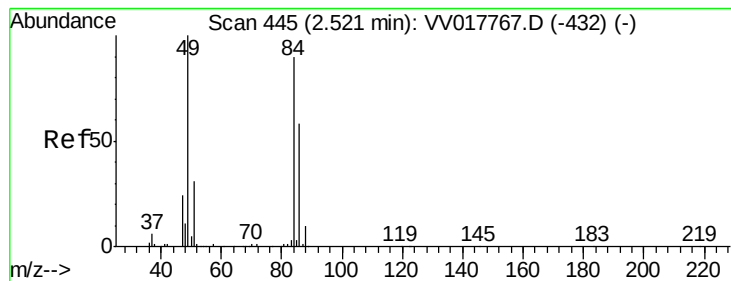

#16
Methylene chloride
Concen: 0.413 ug/L
RT: 2.52 min Scan# 445
Delta R.T. 0.00 min
Lab File: VV017768.D
Acq: 31 Jul 2020 12:18

Instrument :
MSVOA_V
ClientSampleId :
VBLK31

Tot Ion	Ratio	Lower	Upper
84	100		
86	62.5	46.5	86.3
49	109.0	79.2	147.2

