

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017781.D
 Acq On : 31 Jul 2020 17:59
 Operator : SY/MD
 Sample : L3520-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 D0AB8

Quant Time: Aug 01 06:05:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	147506	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	143212	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	73180	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27219	3.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.20%
7) Chloroethane-d5	1.58	69	25498	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.60%
11) 1,1-Dichloroethene-d2	2.12	63	46429	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	3.92	46	63572	37.73	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.46%
24) Chloroform-d	4.38	84	67890	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.60%
26) 1,2-Dichloroethane-d4	5.06	65	39762	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
32) Benzene-d6	5.08	84	117634	3.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.60%
36) 1,2-Dichloropropane-d6	6.10	67	31426	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.60%
41) Toluene-d8	7.34	98	102749	3.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.80%#
45) trans-1,3-Dichloropropene-	7.65	79	13537	3.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.00%
48) 2-Hexanone-d5	8.11	63	41478	33.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.30%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	21965	3.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	46949	4.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.80%


Target Compounds					Ovalue
25) Chloroform	4.40	83	6328	0.310 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017781.D
Acq On : 31 Jul 2020 17:59
Operator : SY/MD
Sample : L3520-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AB8

Quant Time: Aug 01 06:05:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 01 04:42:38 2020
Response via : Initial Calibration

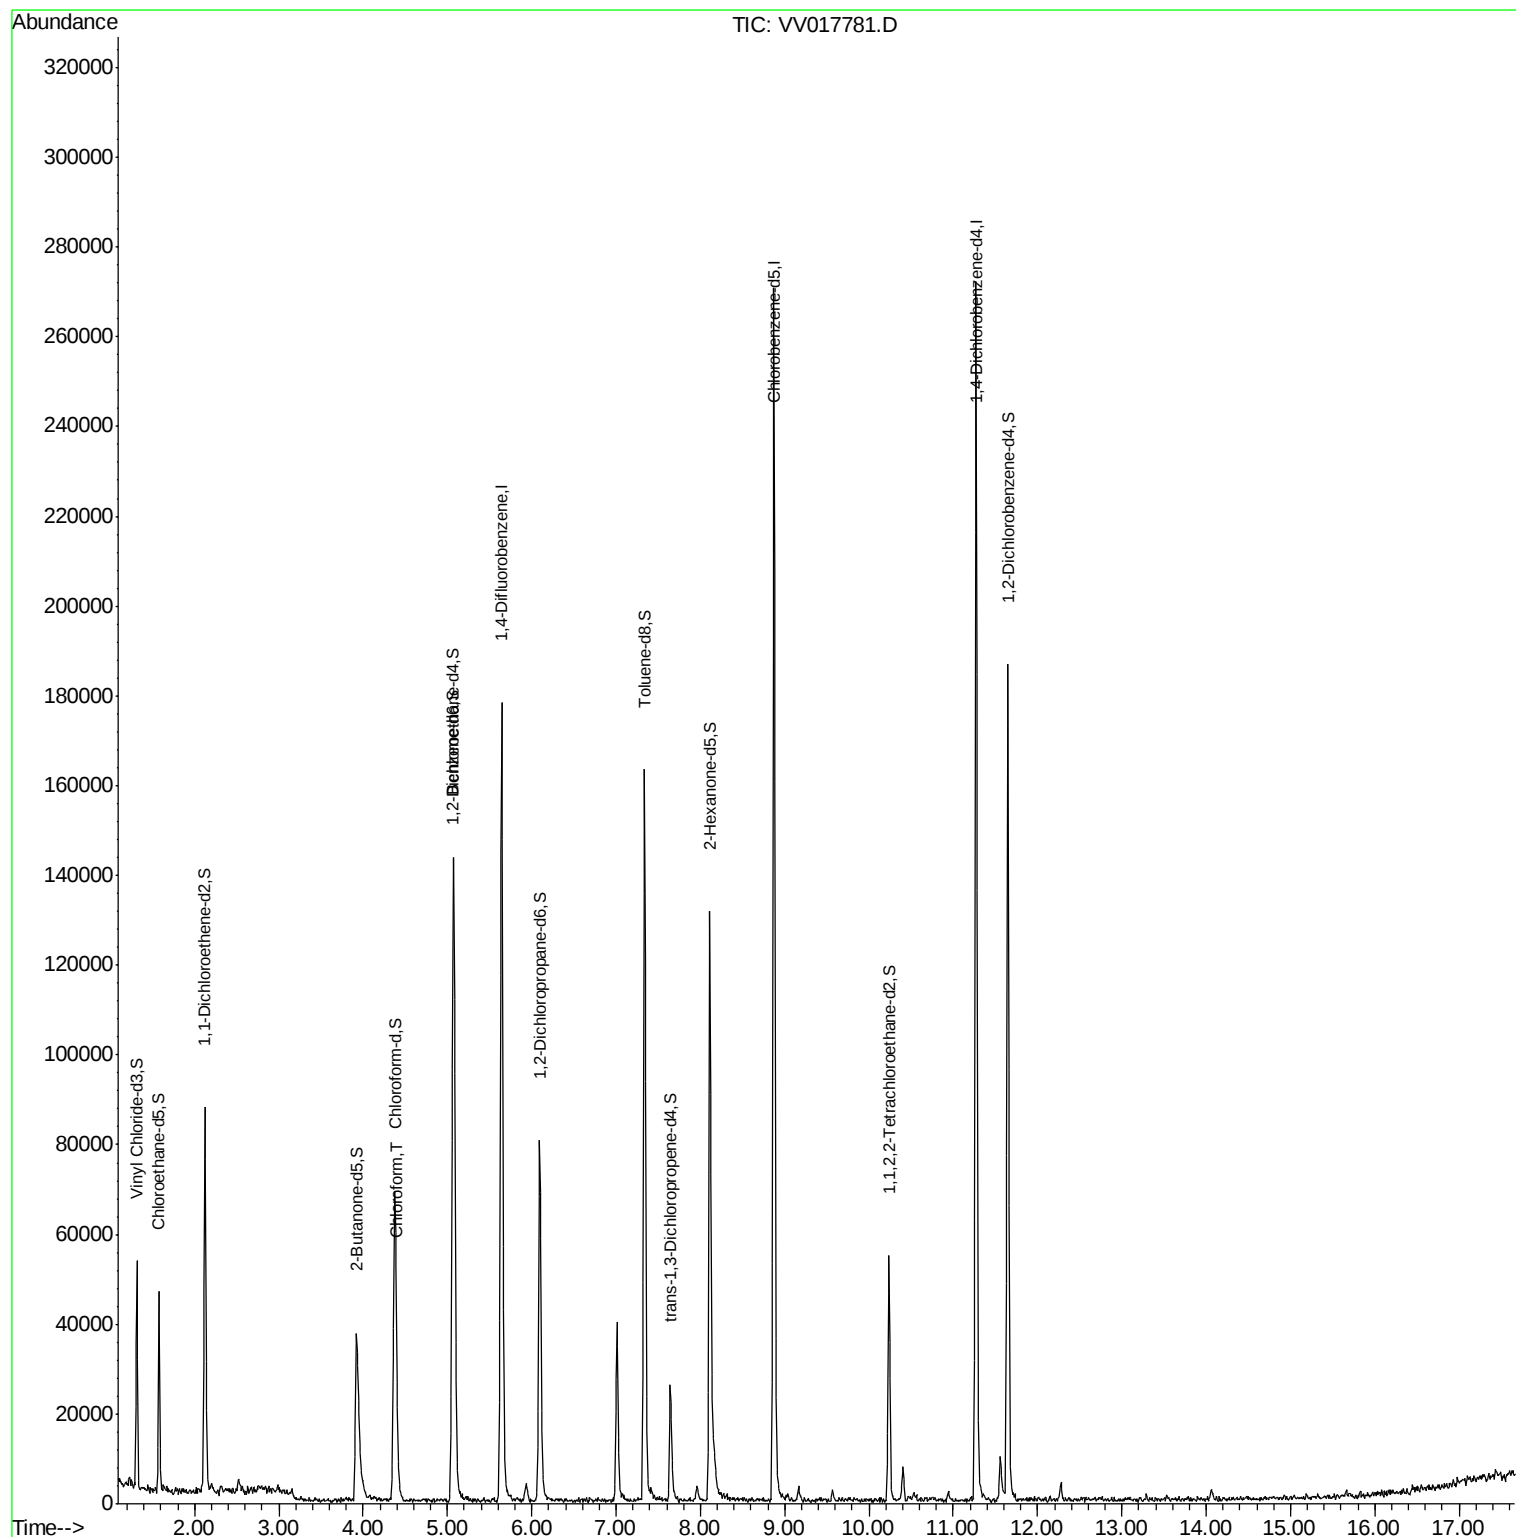

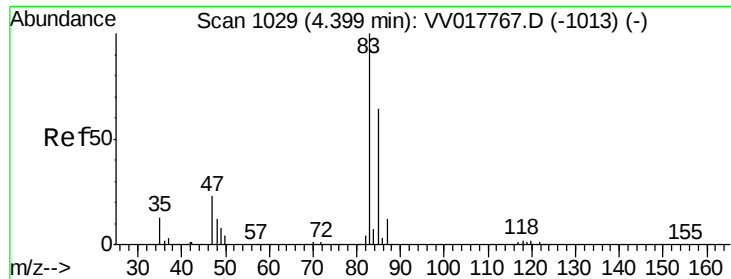

#25
 Chloroform
 Concen: 0.310 ug/L
 RT: 4.40 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VV017781.D
 Acq: 31 Jul 2020 17:59

Instrument :
 MSVOA_V
 ClientSampleId :
 D0AB8

Tot Ion: 83 Resp: 6328
 Ion Ratio Lower Upper
 83 100
 85 67.7 47.3 87.9

