

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017771.D
 Acq On : 31 Jul 2020 13:34
 Operator : SY/MD
 Sample : L3520-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 D0AB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	61	70	78	rBV	54623	56512	13.00%	1.548%
2	1.579	143	152	161	rBV	47876	56620	13.03%	1.551%
3	2.122	309	321	331	rBV	94062	138600	31.89%	3.797%
4	2.196	335	344	349	rBV2	9493	15980	3.68%	0.438%
5	2.528	431	447	456	rBV7	6168	13266	3.05%	0.363%
6	3.926	870	882	906	rBV2	39717	130565	30.04%	3.577%
7	4.376	1007	1022	1045	rBV	80945	198595	45.69%	5.441%
8	5.071	1220	1238	1259	rBV3	161141	397296	91.40%	10.885%
9	5.643	1403	1416	1435	rBV	172264	346697	79.76%	9.499%
10	5.933	1496	1506	1510	rBV7	3863	6089	1.40%	0.167%
11	6.096	1542	1557	1575	rBV2	89554	183943	42.32%	5.040%
12	7.010	1830	1841	1858	rBV2	46291	85290	19.62%	2.337%
13	7.338	1931	1943	1959	rBV	185134	321078	73.87%	8.797%
14	7.643	2029	2038	2053	rBV3	28233	49492	11.39%	1.356%
15	7.958	2124	2136	2146	rBV2	8975	15353	3.53%	0.421%
16	8.109	2174	2183	2217	rBV2	151149	300877	69.22%	8.243%
17	8.875	2407	2421	2441	rBV	259865	430722	99.09%	11.801%
18	10.238	2834	2845	2860	rVB2	62723	96807	22.27%	2.652%
19	10.405	2886	2897	2907	rBV3	22070	36476	8.39%	0.999%
20	11.270	3155	3166	3183	rBV	274665	434668	100.00%	11.909%
21	11.646	3271	3283	3303	rBV	198575	322398	74.17%	8.833%
22	12.276	3469	3479	3489	rBV2	7648	12676	2.92%	0.347%


Sum of corrected areas: 3650000

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017771.D
Acq On : 31 Jul 2020 13:34
Operator : SY/MD
Sample : L3520-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

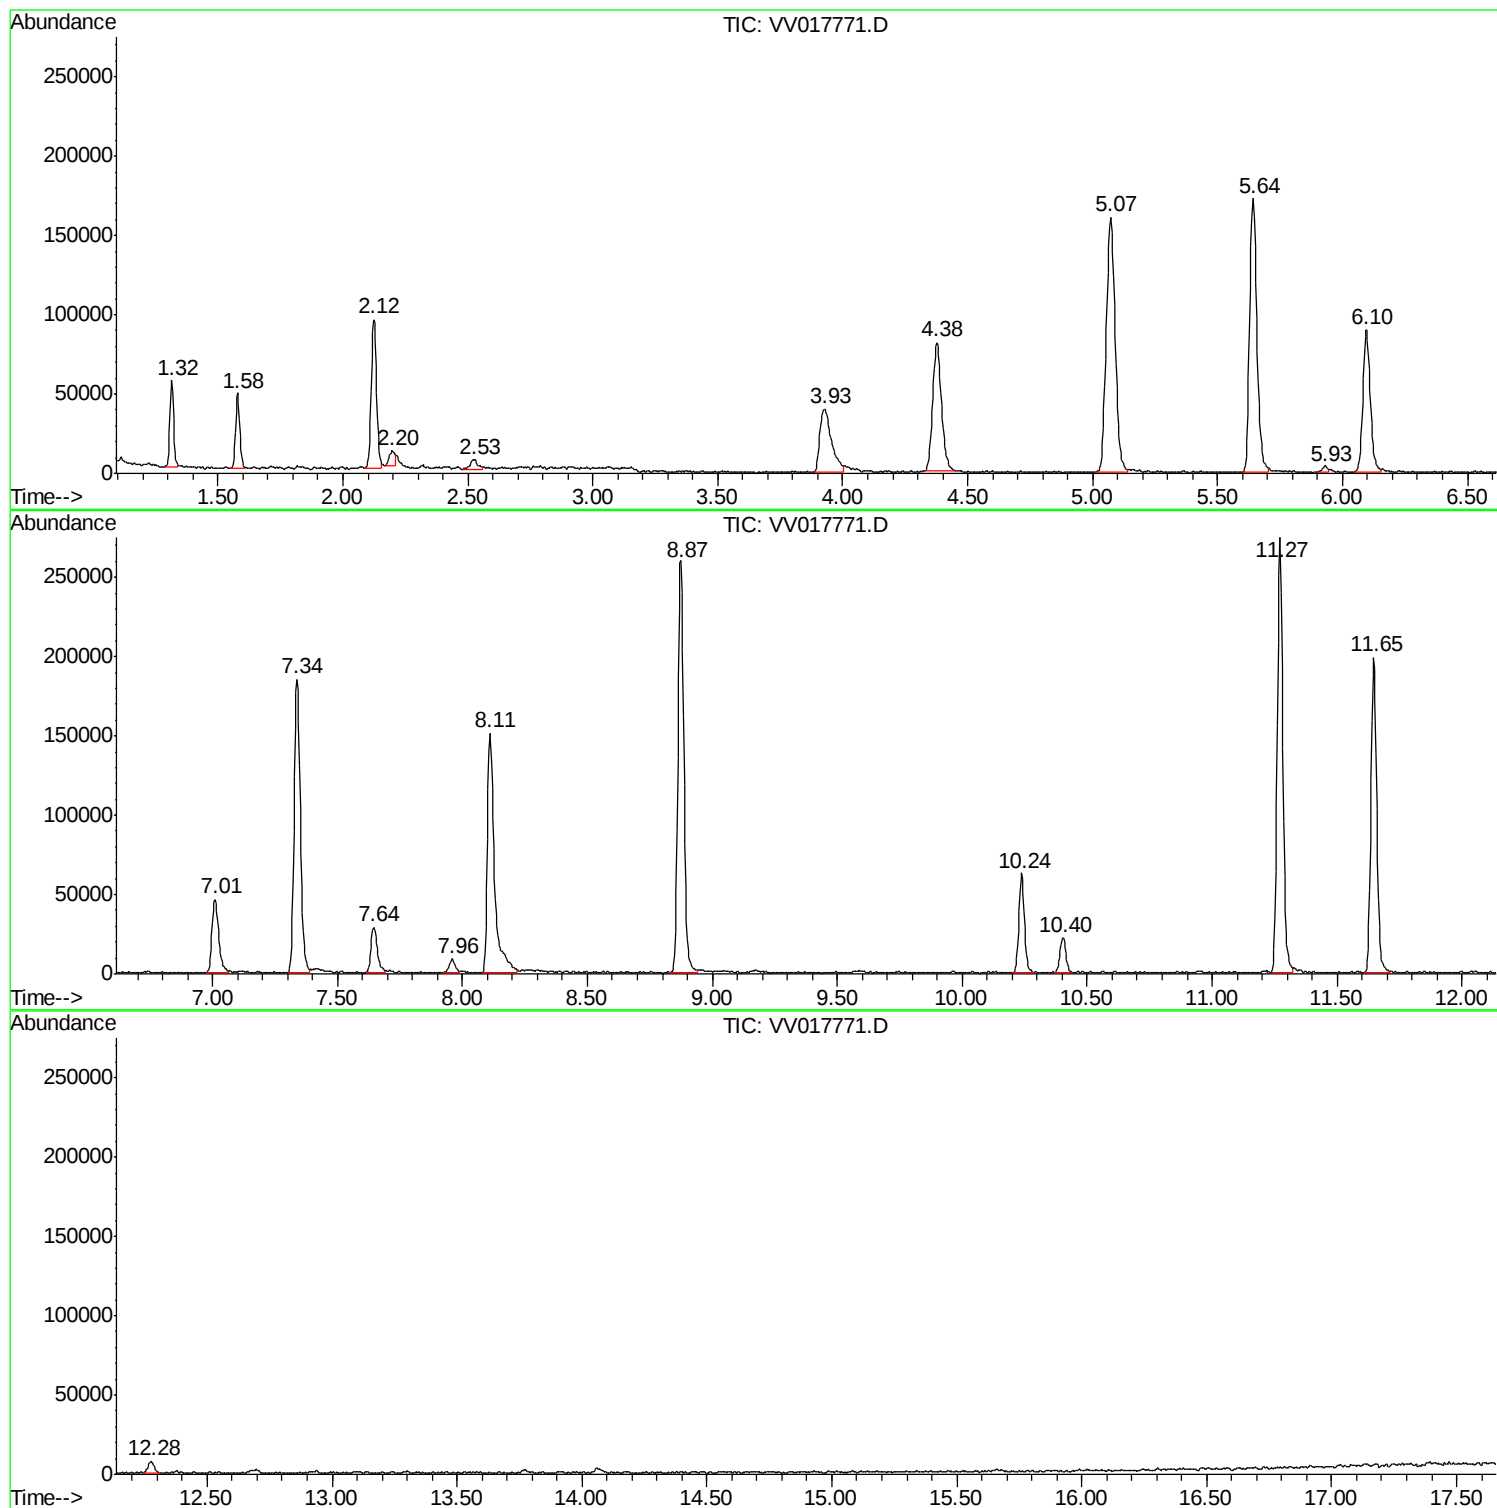

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV073120\
Data File : VV017771.D
Acq On : 31 Jul 2020 13:34
Operator : SY/MD
Sample : L3520-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AB7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV073120\
Data File : VV017771.D
Acq On : 31 Jul 2020 13:34
Operator : SY/MD
Sample : L3520-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AB7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc