

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017786.D
 Acq On : 31 Jul 2020 19:59
 Operator : SY/MD
 Sample : L3520-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	55288	55531	12.97%	1.597%
2	1.579	144	152	160	rVB	45332	51897	12.12%	1.492%
3	2.122	311	321	337	rBV	89032	137284	32.07%	3.947%
4	2.521	436	445	457	rBV	8927	15356	3.59%	0.441%
5	3.926	869	882	921	rBV3	40356	167681	39.18%	4.821%
6	4.380	1004	1023	1047	rBV2	73499	186364	43.54%	5.358%
7	5.074	1221	1239	1259	rBV3	150979	374643	87.53%	10.771%
8	5.640	1403	1415	1433	rBV	168547	341047	79.68%	9.805%
9	5.936	1496	1507	1517	rVB8	4052	7858	1.84%	0.226%
10	6.093	1543	1556	1575	rBV2	87140	180237	42.11%	5.182%
11	7.010	1828	1841	1861	rBV2	44093	81523	19.05%	2.344%
12	7.338	1932	1943	1961	rBV	174923	308132	71.99%	8.859%
13	7.643	2029	2038	2052	rBV2	27023	45119	10.54%	1.297%
14	8.112	2174	2184	2200	rBV	139598	264398	61.77%	7.602%
15	8.447	2277	2288	2297	rBV2	8293	14004	3.27%	0.403%
16	8.874	2409	2421	2441	rBV	256084	428026	100.00%	12.306%
17	10.238	2832	2845	2858	rBV	59695	92626	21.64%	2.663%
18	10.402	2887	2896	2907	rVB3	4959	7174	1.68%	0.206%
19	11.270	3154	3166	3187	rBV	262533	415668	97.11%	11.951%
20	11.646	3272	3283	3299	rBV	189951	303615	70.93%	8.729%


Sum of corrected areas: 3478183

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017786.D
Acq On : 31 Jul 2020 19:59
Operator : SY/MD
Sample : L3520-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

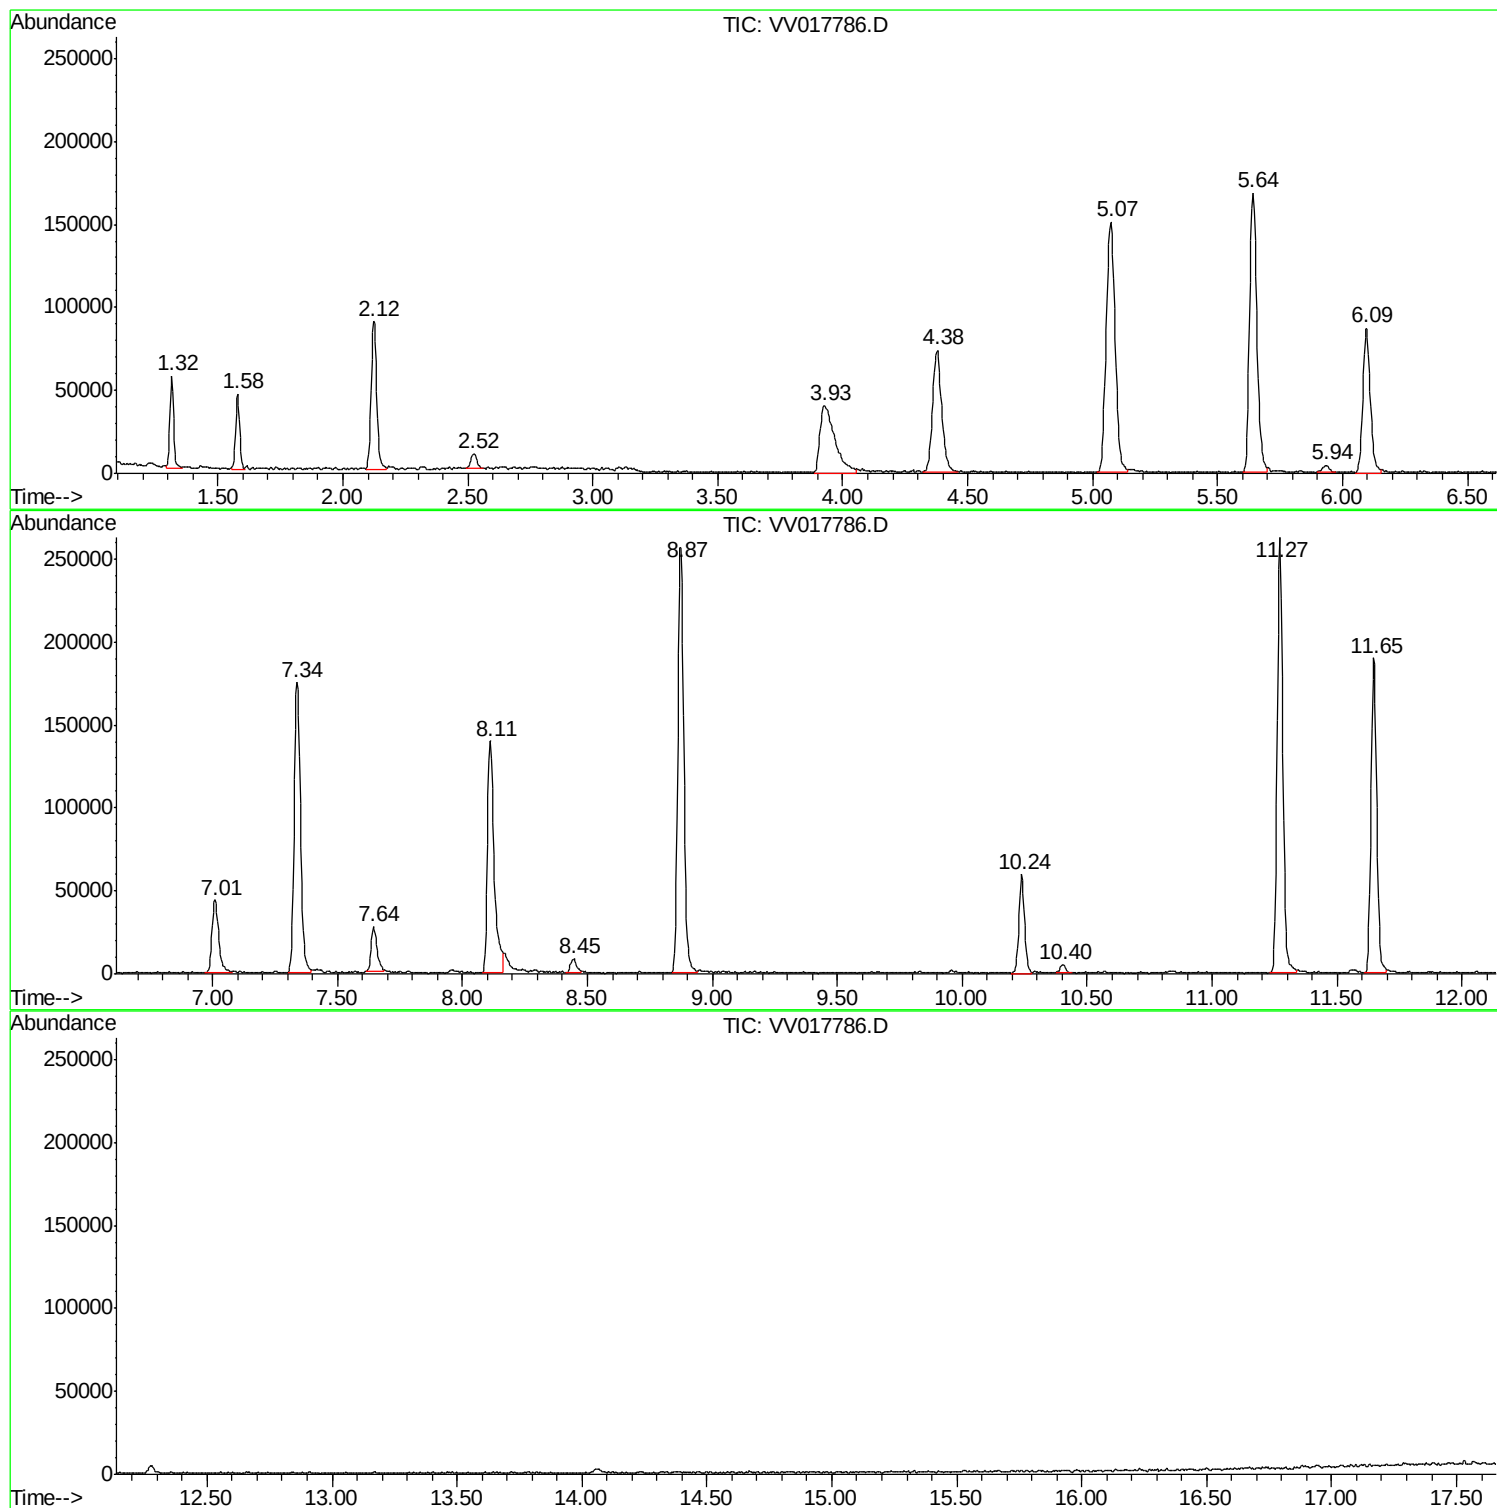

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017786.D
Acq On : 31 Jul 2020 19:59
Operator : SY/MD
Sample : L3520-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.01	1.20 ug/L	81523	1,4-Difluorobenzene	5.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	32
2		.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	25
3		Methane, oxvbis[chloro-	114	C2H4Cl2O	000542-88-1	25
4		1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
5		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25

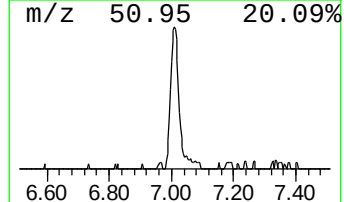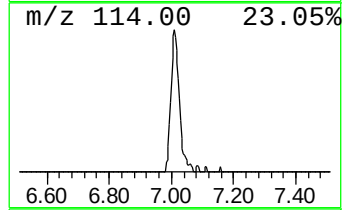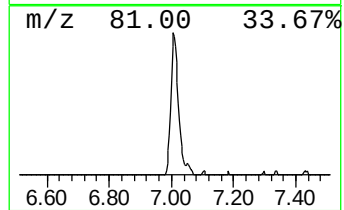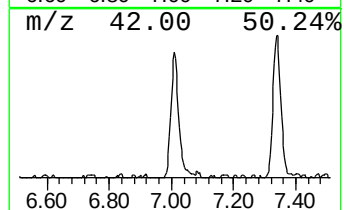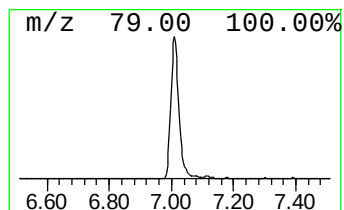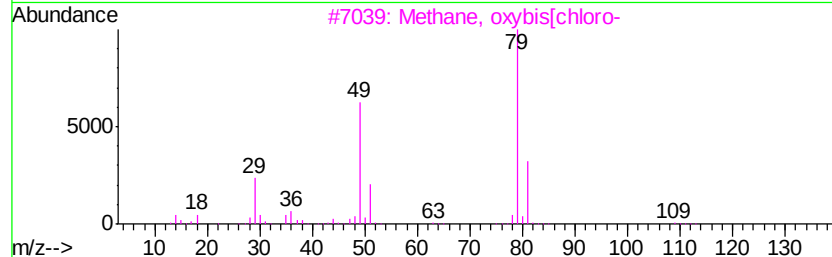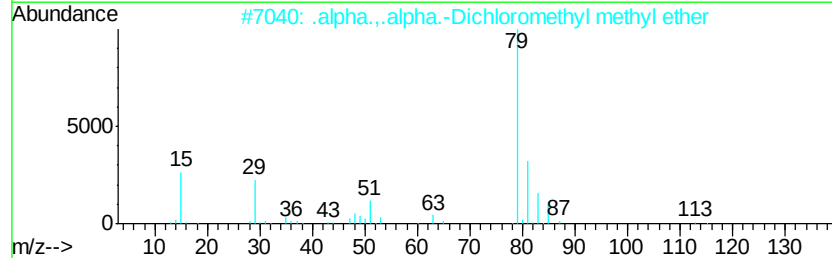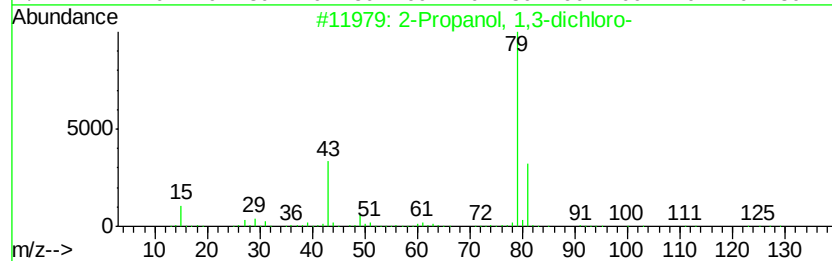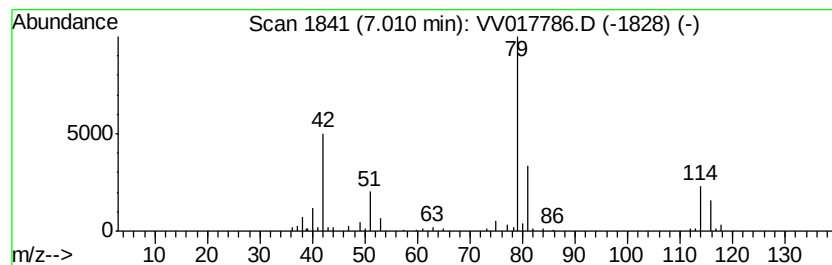

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV073120\
Data File : VV017786.D
Acq On : 31 Jul 2020 19:59
Operator : SY/MD
Sample : L3520-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.01	1.2	ug/L	81523	1	5.64	341047	5.0