


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV073120\
 Data File : VV017766.D
 Acq On : 31 Jul 2020 09:08
 Operator : SY/MD
 Sample : BFB56
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Aug 01 04:42:38 2020

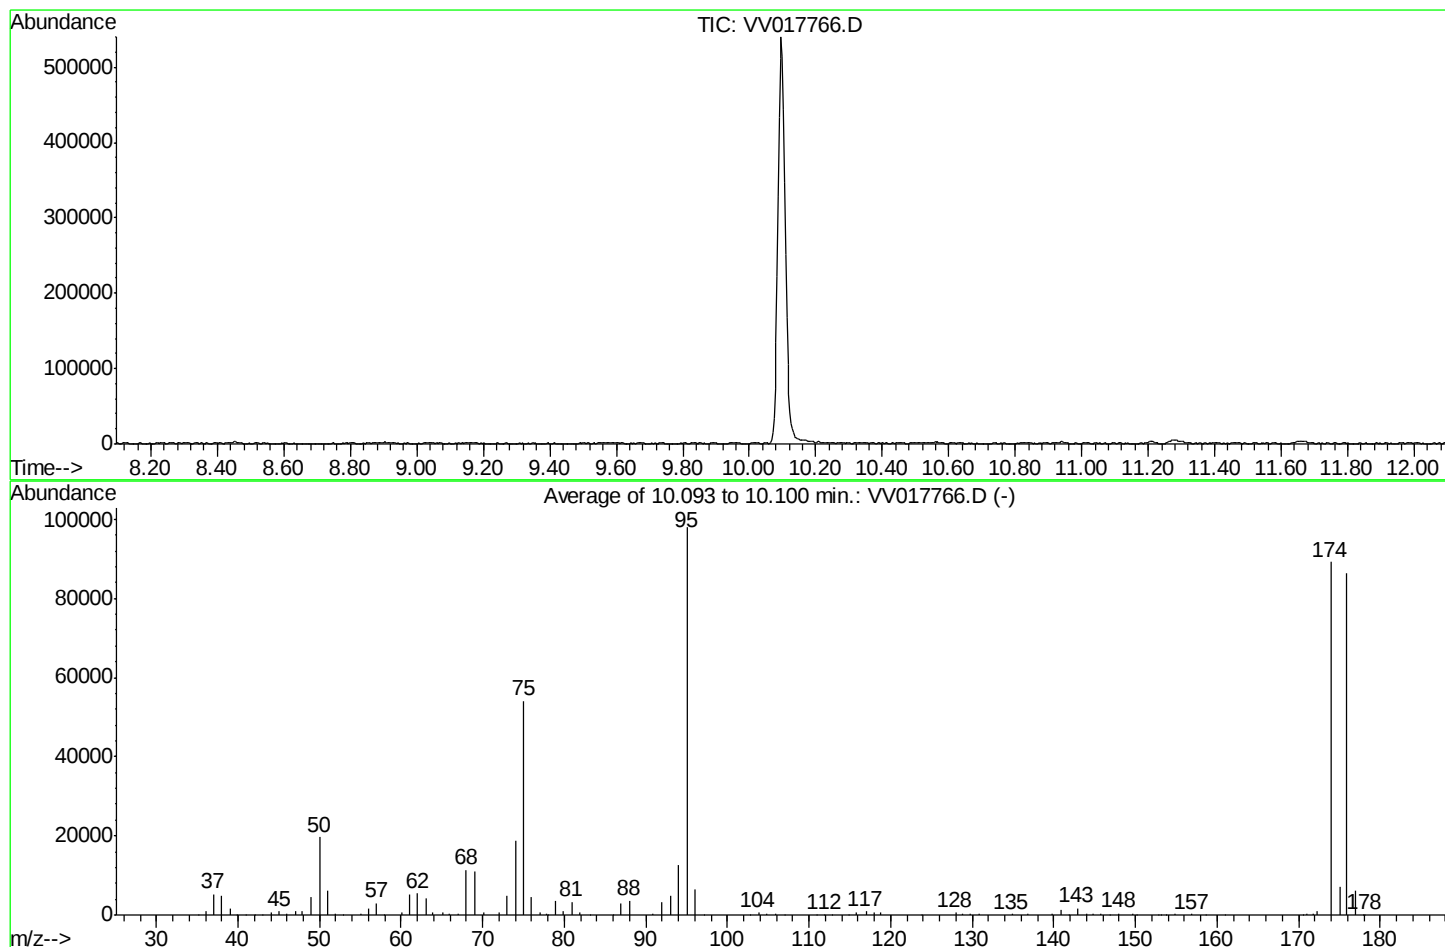

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	19640	PASS
75	95	30	80	55.2	54045	PASS
95	95	100	100	100.0	97952	PASS
96	95	5	9	6.8	6617	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.1	89192	PASS
175	174	5	9	8.1	7253	PASS
176	174	95	101	96.9	86410	PASS
177	176	5	9	7.2	6221	PASS

m/z	Abundance
36.00	1053.0
37.00	5235.0
38.00	4603.0
39.00	1645.0
40.00	256.0
40.90	170.0
42.00	157.0
43.00	118.0
44.00	715.0
45.10	999.0
46.00	228.0
47.10	758.0
47.90	961.0
49.00	4575.0
50.00	19328.0
51.00	6200.0
51.90	366.0
52.90	155.0
54.90	320.0
56.00	1537.0
57.00	2978.0
57.90	154.0
60.10	848.0
61.00	5301.0
62.00	5606.0
63.00	3975.0
63.90	609.0
65.10	852.0
65.90	202.0
67.00	309.0
68.00	11319.0
69.00	11093.0
70.00	873.0
72.00	573.0
73.00	4484.0
74.00	18312.0
75.00	54096.0
76.00	4610.0
77.10	608.0
77.90	380.0
78.00	376.0
78.90	3416.0
79.90	889.0
80.90	3448.0
81.90	670.0
86.90	2885.0
88.00	3378.0
90.90	480.0
92.00	3023.0
93.00	4788.0
94.00	12678.0
95.00	95704.0
96.00	6492.0
97.10	204.0
103.80	522.0
104.90	227.0
105.80	511.0
107.00	153.0
110.90	103.0
111.90	151.0
112.80	132.0
114.90	138.0
115.80	526.0
116.90	828.0
117.90	595.0
118.80	650.0
123.80	111.0
128.00	476.0
128.80	205.0
129.80	457.0
130.80	147.0
134.90	189.0
136.80	253.0
139.90	173.0
140.90	1306.0
141.80	108.0
142.90	1751.0
144.00	156.0
144.80	438.0
145.70	186.0
147.00	174.0
147.90	360.0
149.70	207.0
150.20	131.0
152.80	158.0
153.70	109.0
154.80	215.0
156.90	220.0
158.60	133.0
160.90	164.0
170.40	100.0
171.10	364.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

171.80	649.0
172.30	956.0
173.90	85104.0
175.00	7135.0
175.90	82720.0
177.00	6264.0
178.10	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.10	122.0
36.00	1174.0
37.00	5575.0
38.00	4996.0
39.00	1836.0
40.00	267.0
40.90	148.0
42.00	160.0
43.00	114.0
44.00	758.0
45.10	896.0
46.00	215.0
47.10	868.0
47.90	849.0
49.00	4691.0
50.00	20344.0
51.00	6276.0
52.00	324.0
52.90	154.0
55.00	302.0
56.00	1551.0
57.00	3065.0
57.90	126.0
60.10	799.0
61.00	5521.0
62.00	5706.0
63.00	4199.0
63.90	653.0
65.00	839.0
65.90	219.0
67.00	236.0
68.00	11712.0
69.00	11528.0
70.00	776.0
71.90	640.0
73.00	4888.0
74.00	19552.0
75.00	55896.0
76.00	4523.0
77.10	665.0
77.80	467.0
78.90	3512.0
79.90	1012.0
80.90	3442.0
81.90	629.0
83.10	144.0
86.00	116.0
86.90	3187.0
88.00	3773.0
90.80	447.0
92.00	3416.0
93.00	4997.0
94.00	13103.0
95.00	101360.0
96.00	6935.0
97.10	138.0
103.80	627.0
104.80	259.0
105.90	514.0
106.90	170.0
111.90	148.0
112.80	125.0
114.80	167.0
115.80	526.0
117.00	875.0
117.90	630.0
118.80	772.0
123.80	103.0
127.90	515.0
128.80	237.0
129.80	480.0
130.80	199.0
134.90	297.0
136.80	293.0
139.80	191.0
140.90	1433.0
142.90	1832.0
143.90	204.0
144.80	473.0
145.70	214.0
146.90	151.0
147.90	363.0
149.70	252.0
152.90	128.0
154.80	262.0
156.90	288.0
158.60	154.0
160.90	175.0
171.00	317.0
172.30	944.0
173.90	92088.0
175.00	7457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

175.90	89696.0
177.00	6492.0
177.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	1147.0
37.00	5128.0
38.00	4712.0
39.00	1861.0
39.90	243.0
40.90	119.0
42.00	107.0
44.00	714.0
45.00	699.0
45.90	199.0
47.10	863.0
47.90	674.0
49.00	4354.0
50.00	19248.0
51.00	5643.0
52.10	252.0
52.90	140.0
55.10	283.0
56.00	1433.0
57.00	2728.0
58.00	114.0
60.00	803.0
61.00	5134.0
62.00	5105.0
63.00	4126.0
63.90	543.0
65.00	682.0
65.80	181.0
68.00	11122.0
69.00	10810.0
70.10	605.0
71.90	594.0
73.00	4759.0
74.00	18672.0
75.00	52144.0
76.00	4176.0
77.10	645.0
77.80	368.0
78.90	3340.0
79.90	1019.0
80.90	3309.0
82.00	628.0
83.10	175.0
86.90	3113.0
88.00	3612.0
90.80	433.0
92.00	3341.0
93.00	4676.0
94.00	12335.0
95.00	96792.0
96.00	6426.0
97.10	108.0
102.80	100.0
103.80	618.0
104.80	235.0
105.90	449.0
106.90	161.0
111.90	128.0
114.70	173.0
115.90	468.0
117.00	791.0
117.90	536.0
118.80	752.0
127.90	515.0
128.90	235.0
129.70	501.0
130.90	210.0
134.90	351.0
136.80	283.0
139.70	173.0
140.90	1411.0
142.90	1741.0
143.90	220.0
144.90	402.0
145.80	179.0
146.80	113.0
148.00	295.0
149.70	242.0
153.10	136.0
154.80	329.0
156.90	361.0
158.70	197.0
160.90	160.0
170.50	190.0
170.90	248.0
172.20	954.0
173.90	90384.0
175.00	7169.0
175.90	86816.0
177.00	5907.0
177.90	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	112.0
36.60	107.0
39.90	160.0
41.00	117.0
44.00	229.0
64.30	106.0
97.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56