

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006821.D
 Acq On : 02 Aug 2018 21:16
 Operator : SY/MD
 Sample : J4315-10
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KY8

Quant Time: Aug 03 11:35:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 03 01:56:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	74251	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	66753	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	25550	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	73679	14.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	286.40%#
7) Chloroethane-d5	1.58	69	66603	14.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	298.00%#
11) 1,1-Dichloroethene-d2	2.13	63	98966	10.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	207.60%#
20) 2-Butanone-d5	3.96	46	220182	176.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	353.06%#
24) Chloroform-d	4.41	84	135192	15.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	300.40%#
26) 1,2-Dichloroethane-d4	5.09	65	72640	16.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	320.00%#
32) Benzene-d6	5.10	84	267998	14.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	297.40%#
36) 1,2-Dichloropropane-d6	6.12	67	89791	15.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	301.80%#
41) Toluene-d8	7.37	98	205034	12.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	254.80%#
43) trans-1,3-Dichloropropene-	7.67	79	28241	13.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	268.40%#
46) 2-Hexanone-d5	8.14	63	137788	147.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	294.12%#
57) 1,1,2,2-Tetrachloroethane-	10.27	84	75310	17.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	340.20%#
64) 1,2-Dichlorobenzene-d4	11.68	152	69315	14.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	292.40%#


Target Compounds					Ovalue
25) Chloroform	4.43	83	5819	0.62 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080218\
Data File : VV006821.D
Acq On : 02 Aug 2018 21:16
Operator : SY/MD
Sample : J4315-10
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KY8

Quant Time: Aug 03 11:35:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 03 01:56:09 2018
Response via : Initial Calibration

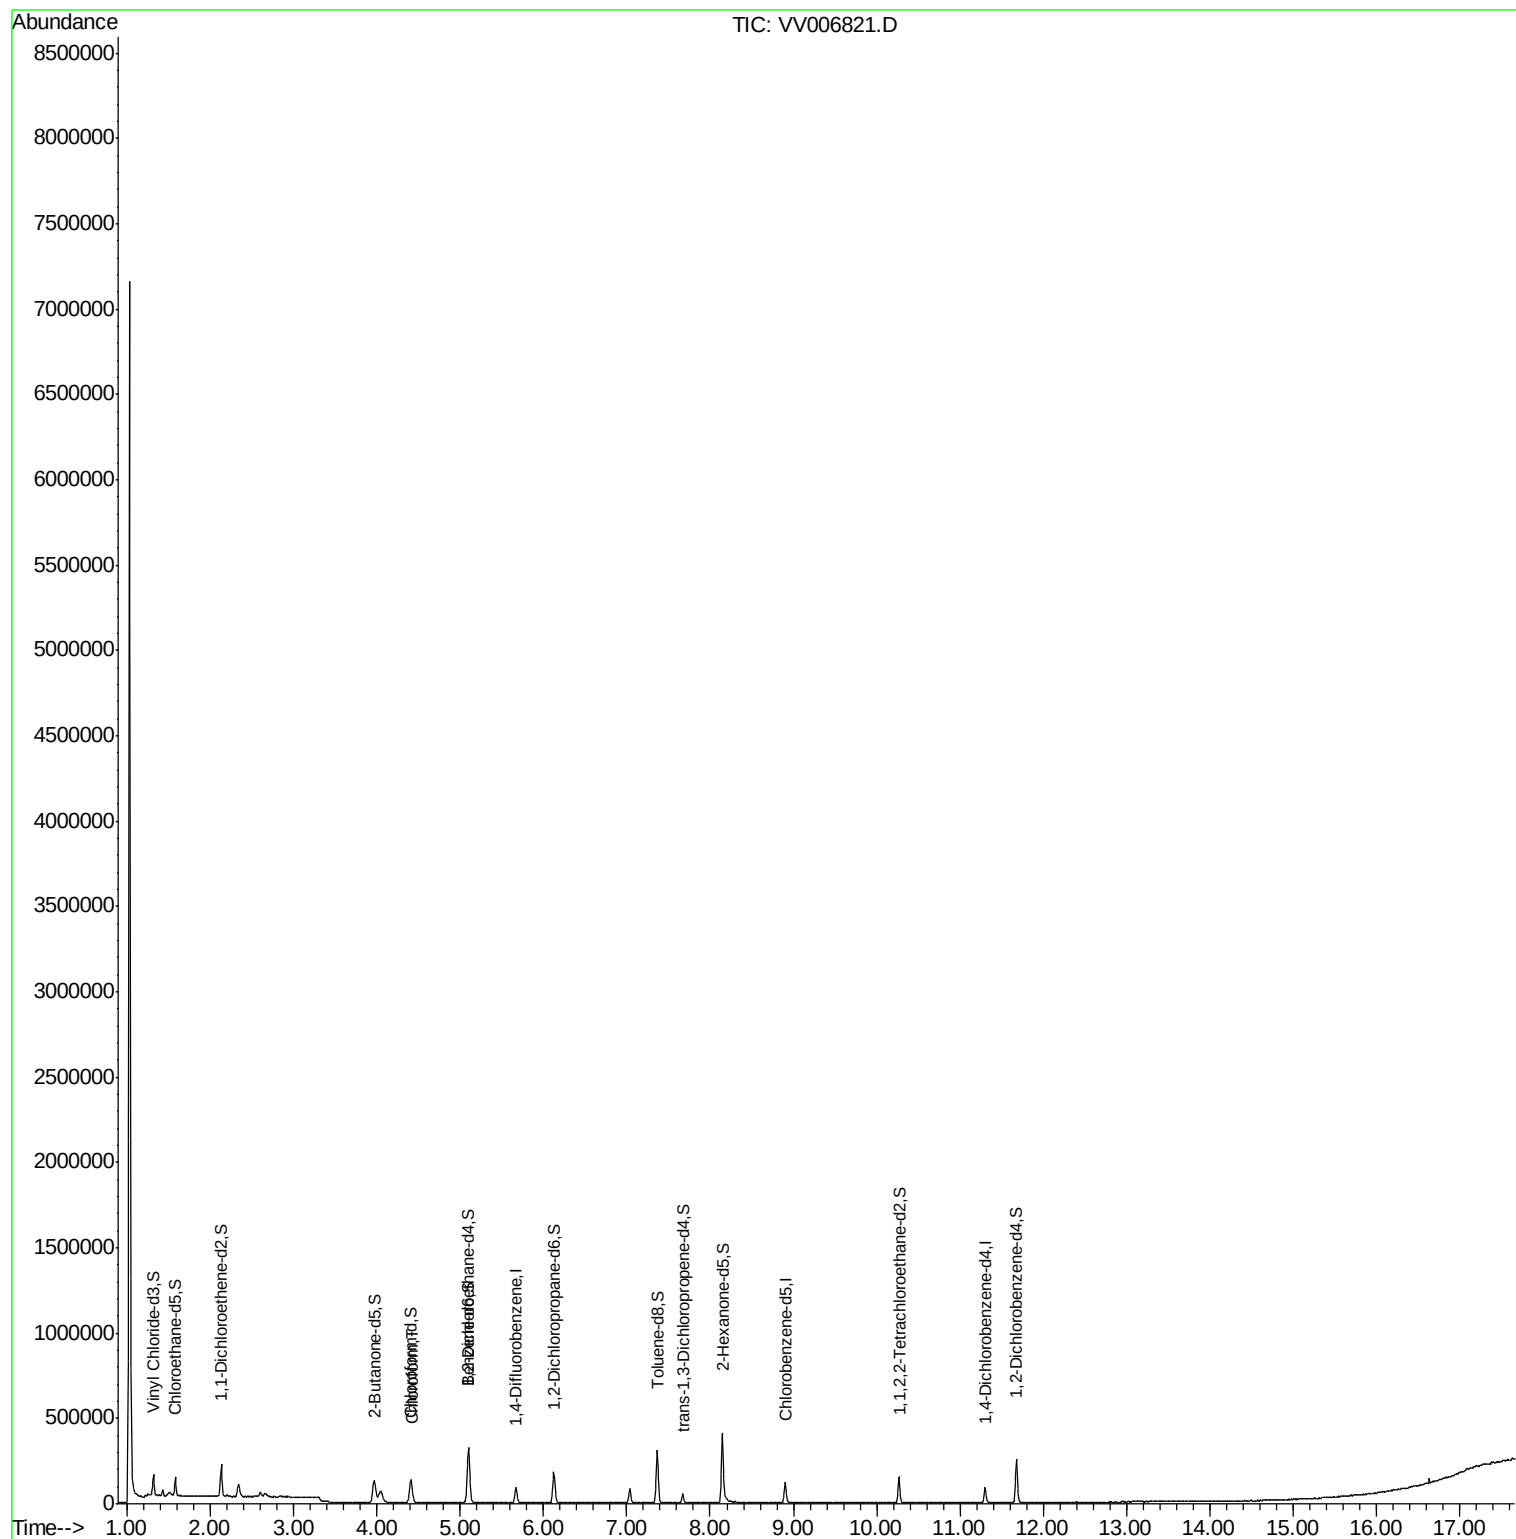

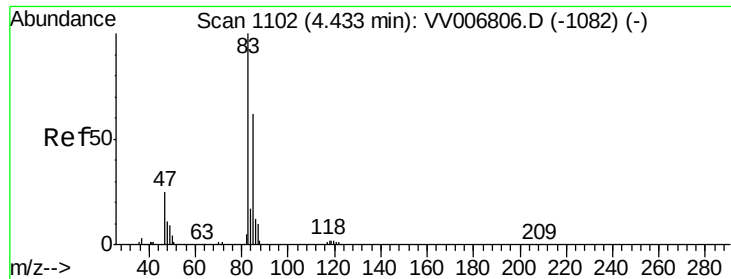

#25
 Chloroform
 Concen: 0.62 ug/L
 RT: 4.43 min Scan# 1101
 Delta R.T. -0.00 min
 Lab File: VV006821.D
 Acq: 02 Aug 2018 21:16

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KY8

Tot Ion: 83 Resp: 5819
 Ion Ratio Lower Upper
 83 100
 85 62.4 45.4 84.2

