

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006832.D
 Acq On : 03 Aug 2018 03:05
 Operator : SY/MD
 Sample : J4261-08
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E5F94

Quant Time: Aug 03 04:29:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 03 04:21:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	213987	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	195920	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	70918	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77978	5.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.20%
7) Chloroethane-d5	1.58	69	74316	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.40%
11) 1,1-Dichloroethene-d2	2.13	63	106099	3.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.20%
20) 2-Butanone-d5	3.95	46	243576	67.76	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	135.52%#
24) Chloroform-d	4.41	84	150111	5.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.80%
26) 1,2-Dichloroethane-d4	5.09	65	81587	6.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.80%
32) Benzene-d6	5.10	84	285112	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
36) 1,2-Dichloropropane-d6	6.12	67	100673	5.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.40%
41) Toluene-d8	7.37	98	215336	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.67	79	29805	4.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.40%
46) 2-Hexanone-d5	8.14	63	152912	55.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.20%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	80597	6.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.00%#
64) 1,2-Dichlorobenzene-d4	11.68	152	73767	5.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	15821	6.24 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
Data File : VV006832.D
Acq On : 03 Aug 2018 03:05
Operator : SY/MD
Sample : J4261-08
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E5F94

Quant Time: Aug 03 04:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 03 04:21:42 2018
Response via : Initial Calibration

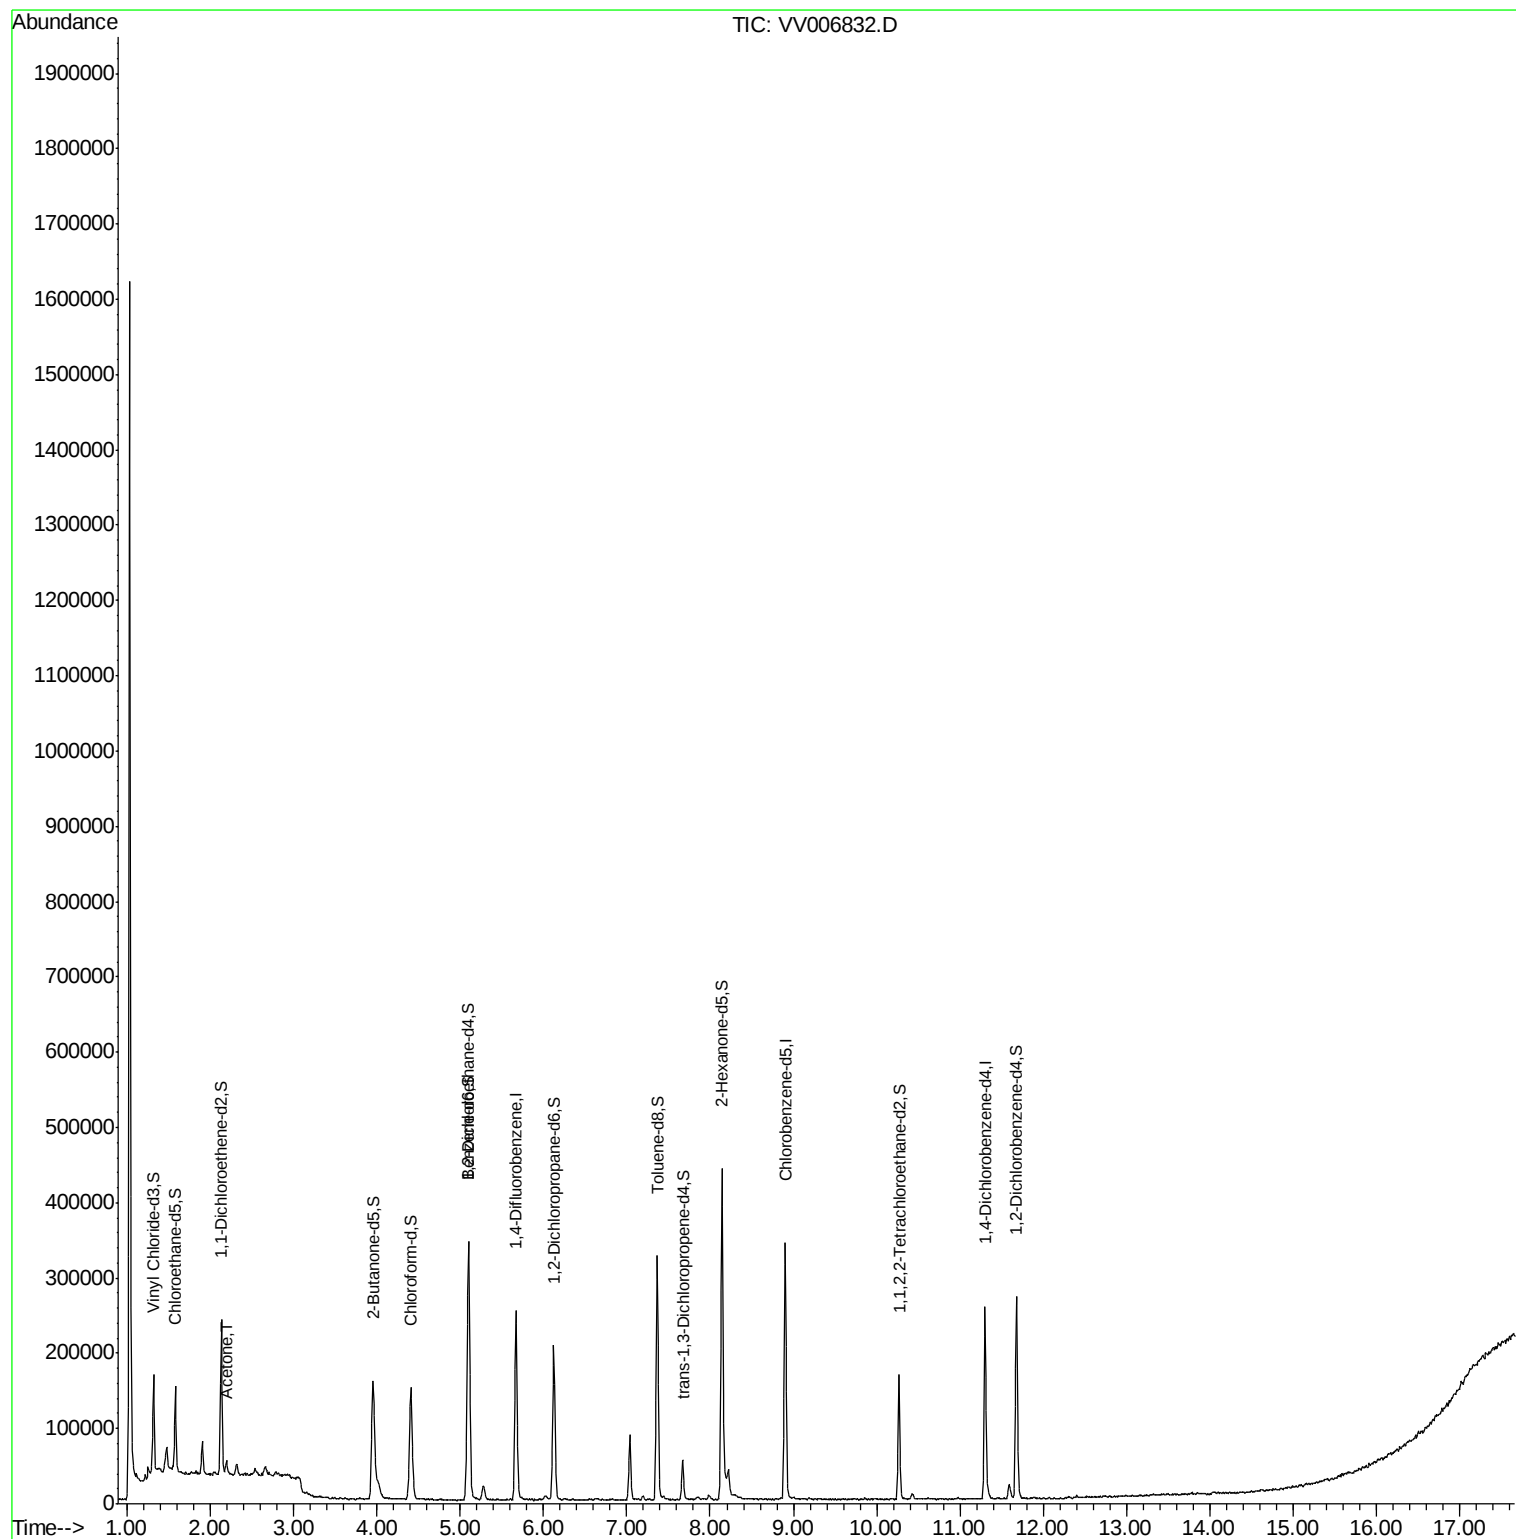

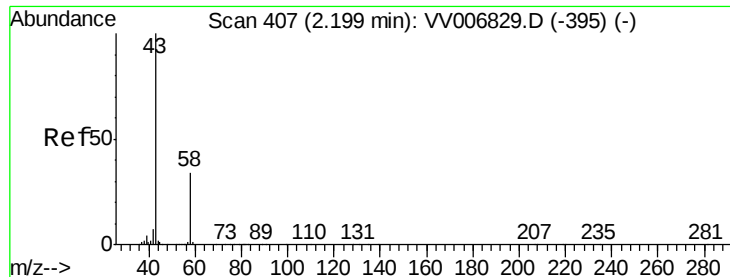

#13

Acetone

Concen: 6.24 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.01 min

Lab File: VV006832.D

Acq: 03 Aug 2018 03:05

Instrument :
MSVOA_V
ClientSampleId :
E5F94

Tot Ion: 43 Resp: 15821

Ion Ratio Lower Upper

43 100

58 38.6 0.0 69.0

