

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006834.D
 Acq On : 03 Aug 2018 03:59
 Operator : SY/MD
 Sample : J4227-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWQ2

Quant Time: Aug 03 04:33:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 03 04:21:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	228304	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	209549	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	77214	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80359	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.58	69	71869	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.60%
11) 1,1-Dichloroethene-d2	2.13	63	109118	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	3.95	46	239257	62.39	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.78%
24) Chloroform-d	4.41	84	144354	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.40%
26) 1,2-Dichloroethane-d4	5.09	65	79161	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.40%
32) Benzene-d6	5.10	84	281898	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.12	67	97705	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	7.37	98	218210	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
43) trans-1,3-Dichloropropene-	7.67	79	29409	4.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.00%
46) 2-Hexanone-d5	8.14	63	145241	49.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	78575	5.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	76392	5.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	13321	4.93 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080218\
Data File : VV006834.D
Acq On : 03 Aug 2018 03:59
Operator : SY/MD
Sample : J4227-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWQ2

Quant Time: Aug 03 04:33:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 03 04:21:42 2018
Response via : Initial Calibration

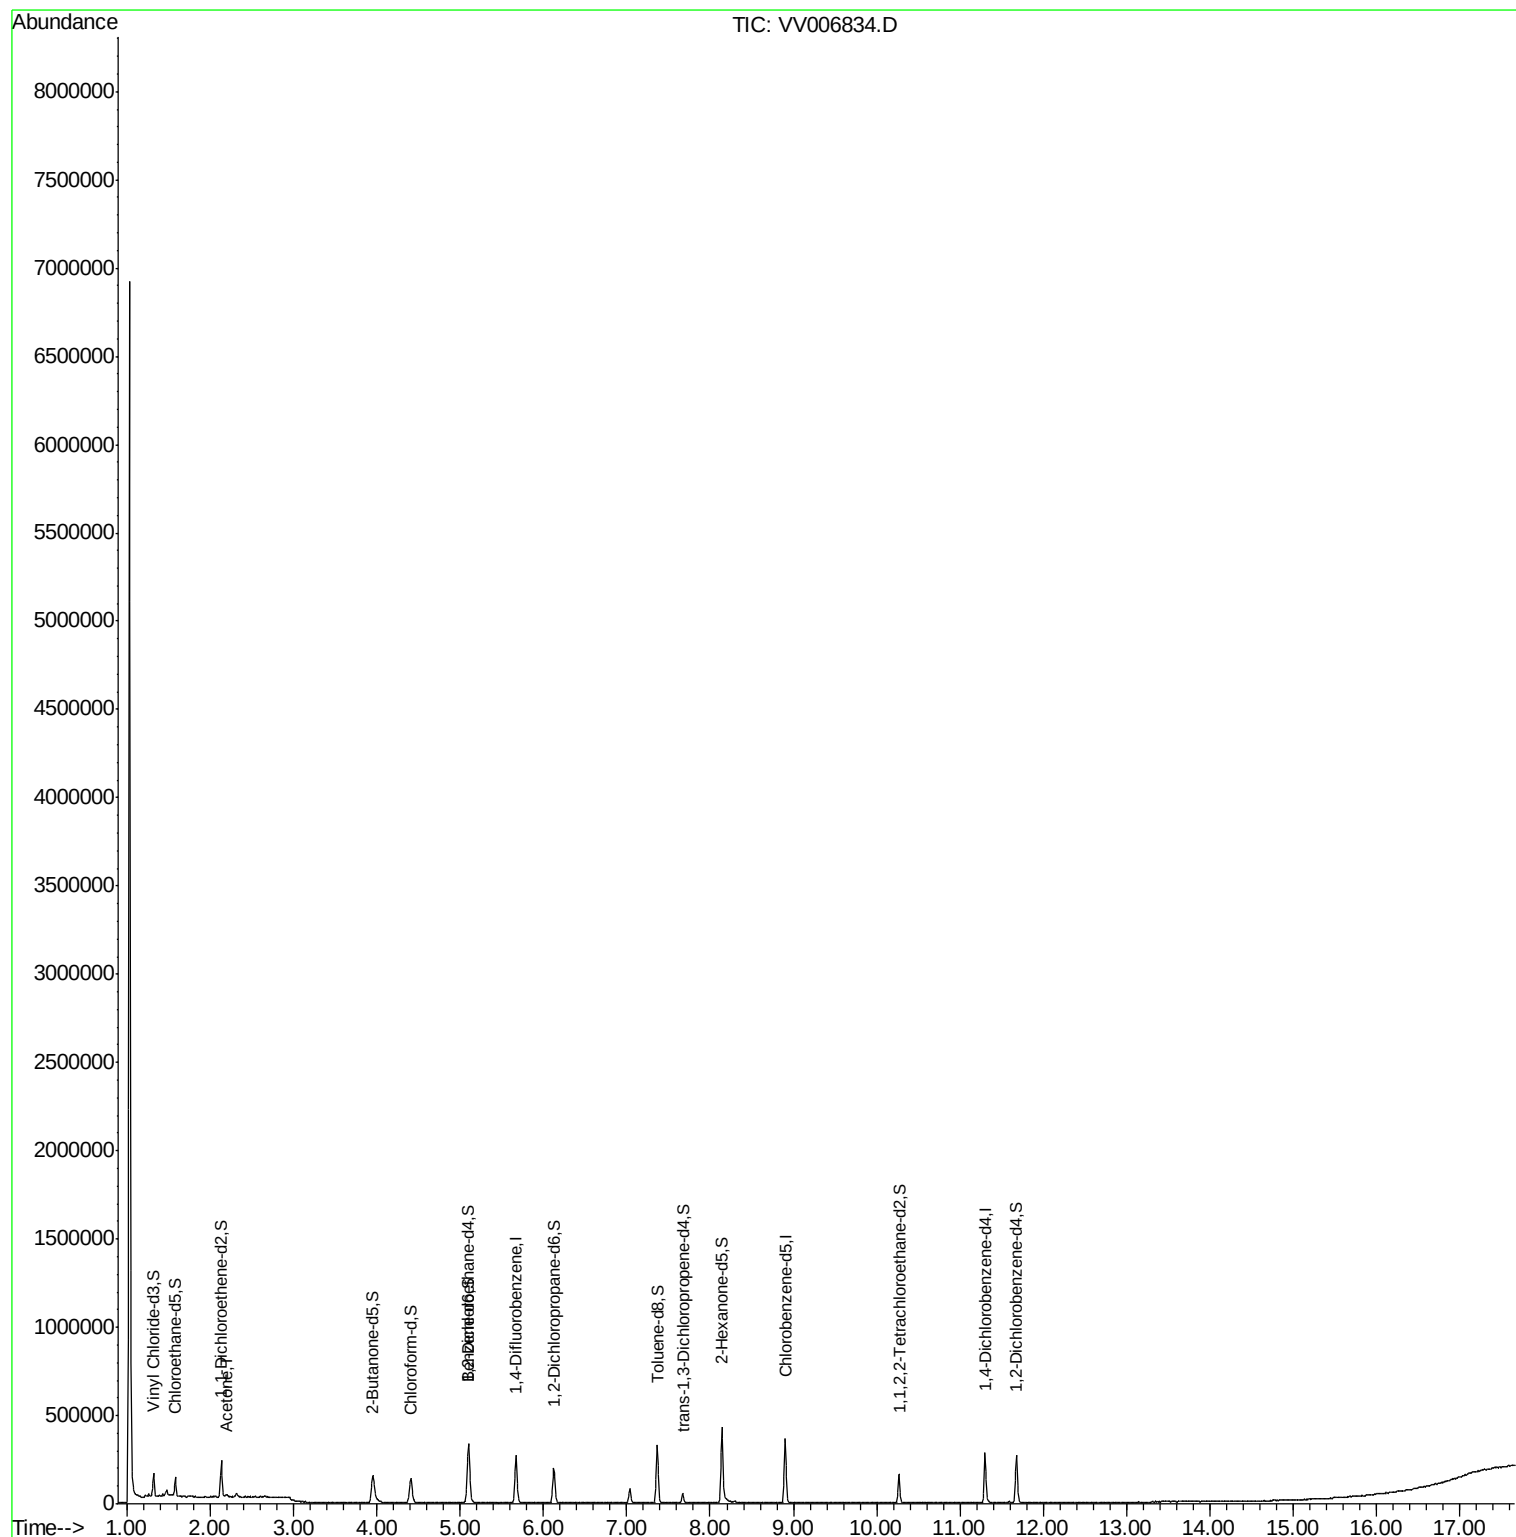

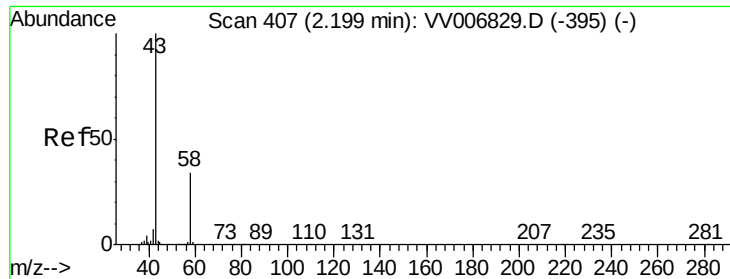

#13

Acetone

Concen: 4.93 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.01 min

Lab File: VV006834.D

Acq: 03 Aug 2018 03:59

Instrument :
MSVOA_V
ClientSampleId :
ESWQ2

Tot Ion: 43 Resp: 13321

Ion Ratio Lower Upper

43 100

58 31.4 0.0 69.0

