

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006837.D
 Acq On : 03 Aug 2018 05:19
 Operator : SY/MD
 Sample : J4227-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWQ5

Quant Time: Aug 03 09:15:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 03 04:21:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	237329	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	215816	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	79551	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	79081	4.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.20%
7) Chloroethane-d5	1.58	69	74224	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.80%
11) 1,1-Dichloroethene-d2	2.13	63	112017	3.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.60%
20) 2-Butanone-d5	3.95	46	234713	58.88	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.76%
24) Chloroform-d	4.41	84	148725	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
26) 1,2-Dichloroethane-d4	5.09	65	78583	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
32) Benzene-d6	5.10	84	285903	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.12	67	99600	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.37	98	220028	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.67	79	28619	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.14	63	144036	47.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	79124	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	74561	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	11727	4.17 ug/L	99
53) m,p-xylene	9.19	106	7354	0.29 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080218\
Data File : VV006837.D
Acq On : 03 Aug 2018 05:19
Operator : SY/MD
Sample : J4227-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWQ5

Quant Time: Aug 03 09:15:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 03 04:21:42 2018
Response via : Initial Calibration




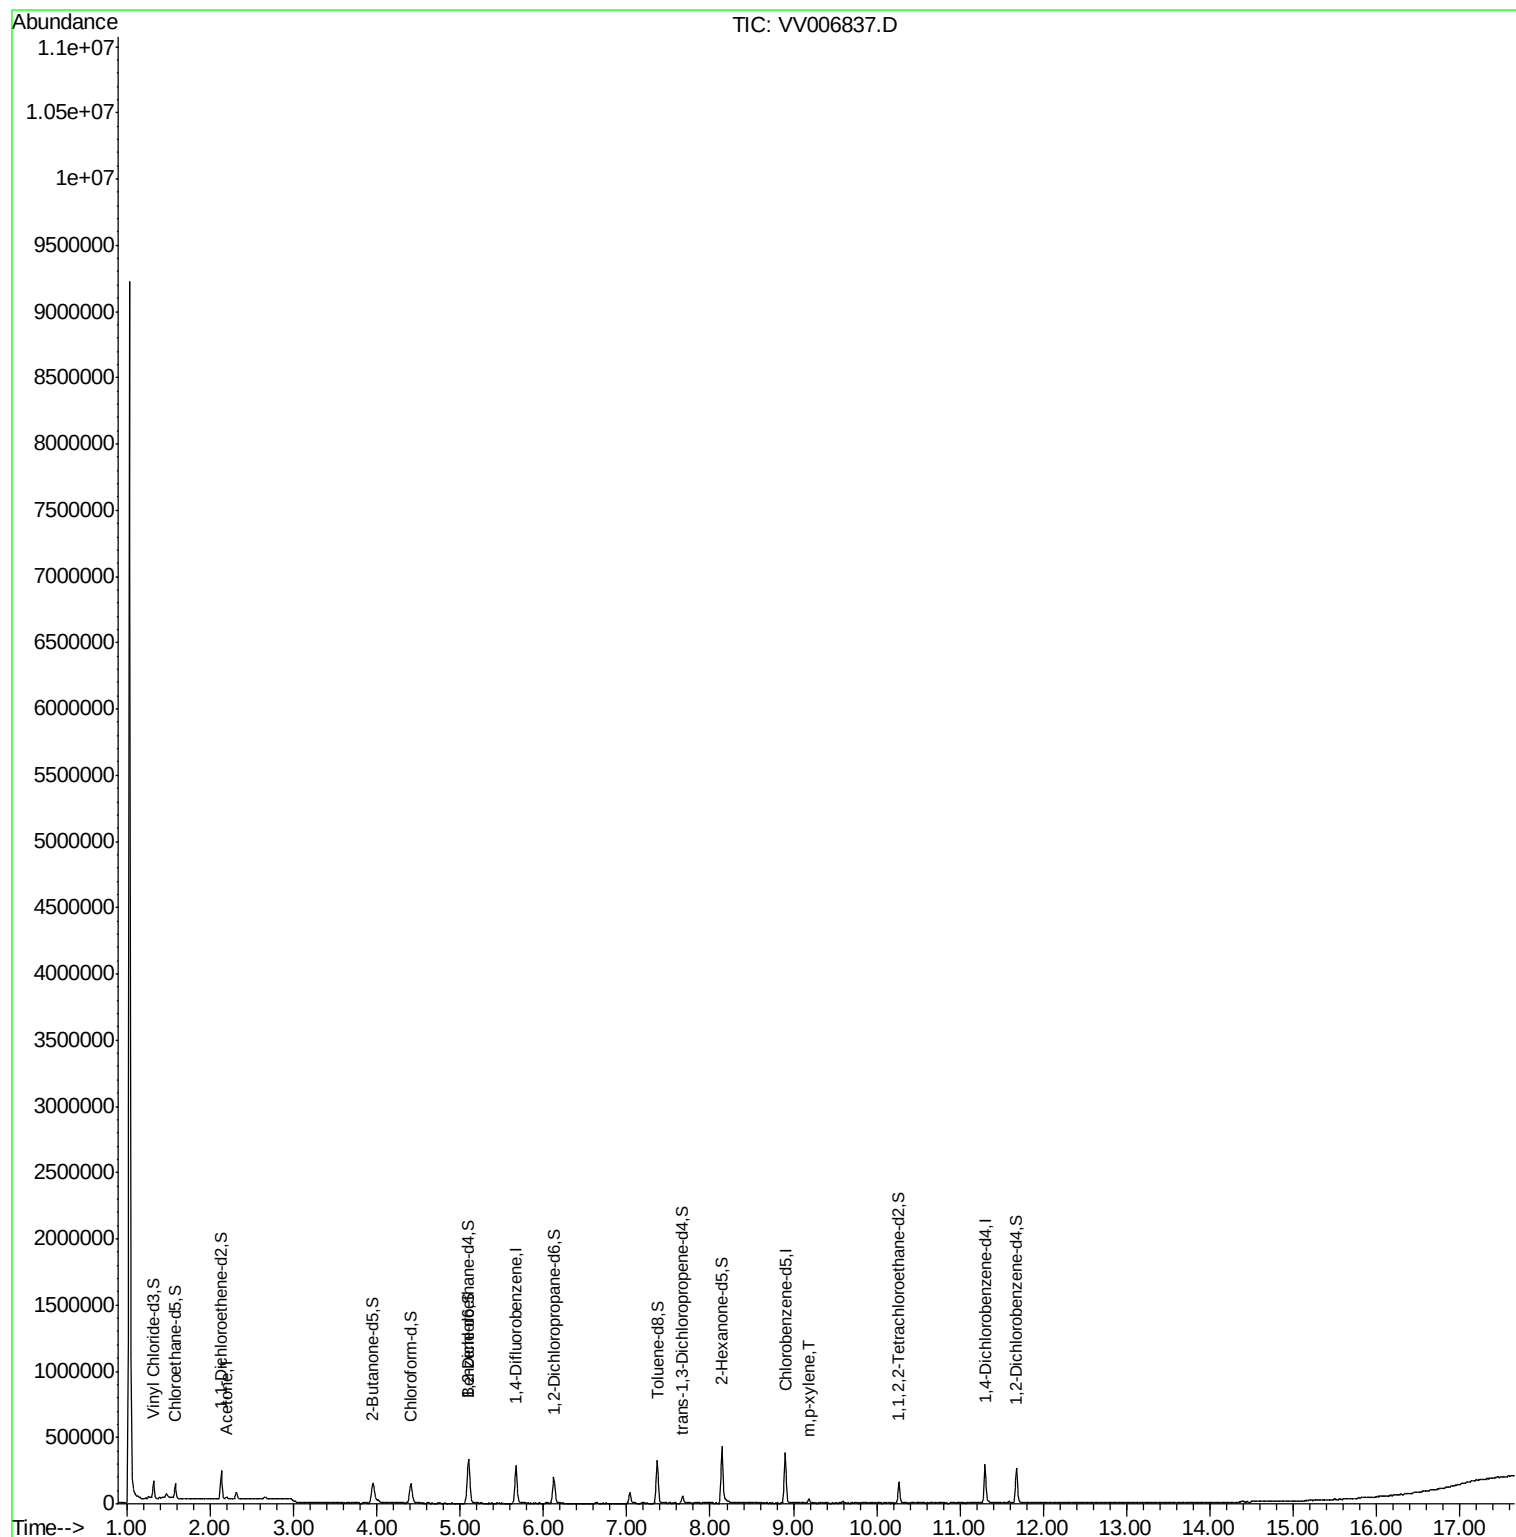


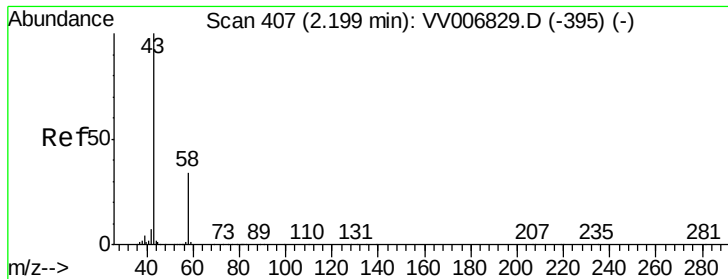

#13
Acetone
Concen: 4.17 ug/L
RT: 2.19 min Scan# 405
Delta R.T. -0.01 min
Lab File: VV006837.D
Acq: 03 Aug 2018 05:19

Instrument :
MSVOA_V
ClientSampleId :
ESWQ5

Tot Ion: 43 Resp: 11727
Ion Ratio Lower Upper
43 100
58 35.2 0.0 69.0

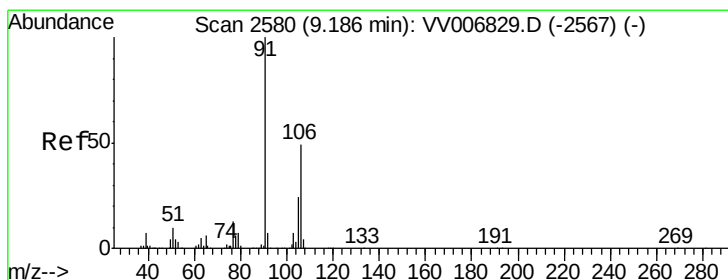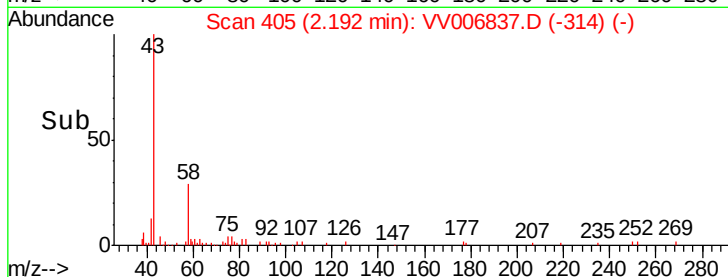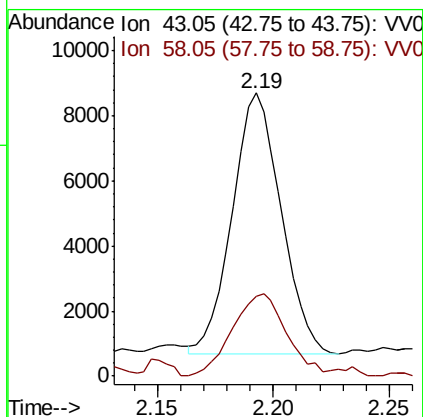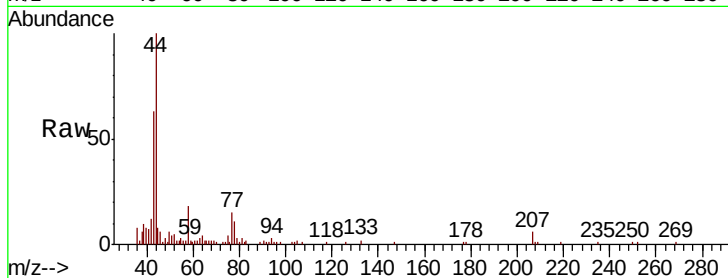

#53
m,p-xylene
Concen: 0.29 ug/L
RT: 9.19 min Scan# 2580
Delta R.T. -0.00 min
Lab File: VV006837.D
Acq: 03 Aug 2018 05:19

Tgt Ion: 106 Resp: 7354
Ion Ratio Lower Upper
106 100
91 207.6 137.4 255.2

