

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006850.D
 Acq On : 03 Aug 2018 11:47
 Operator : SY/MD
 Sample : J4261-21
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E5FA5

Quant Time: Aug 03 12:47:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 03 04:21:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	240179	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	220439	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	82355	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77295	4.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.00%
7) Chloroethane-d5	1.58	69	75361	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.20%
11) 1,1-Dichloroethene-d2	2.13	63	113156	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.95	46	206925	51.29	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.58%
24) Chloroform-d	4.40	84	152153	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
26) 1,2-Dichloroethane-d4	5.09	65	76506	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.20%
32) Benzene-d6	5.10	84	287515	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.12	67	97432	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.37	98	223385	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.00%
43) trans-1,3-Dichloropropene-	7.67	79	30348	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.14	63	123512	39.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.84%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	73027	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	73615	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	17558	0.63 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080218\
Data File : VV006850.D
Acq On : 03 Aug 2018 11:47
Operator : SY/MD
Sample : J4261-21
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E5FA5

Quant Time: Aug 03 12:47:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 03 04:21:42 2018
Response via : Initial Calibration

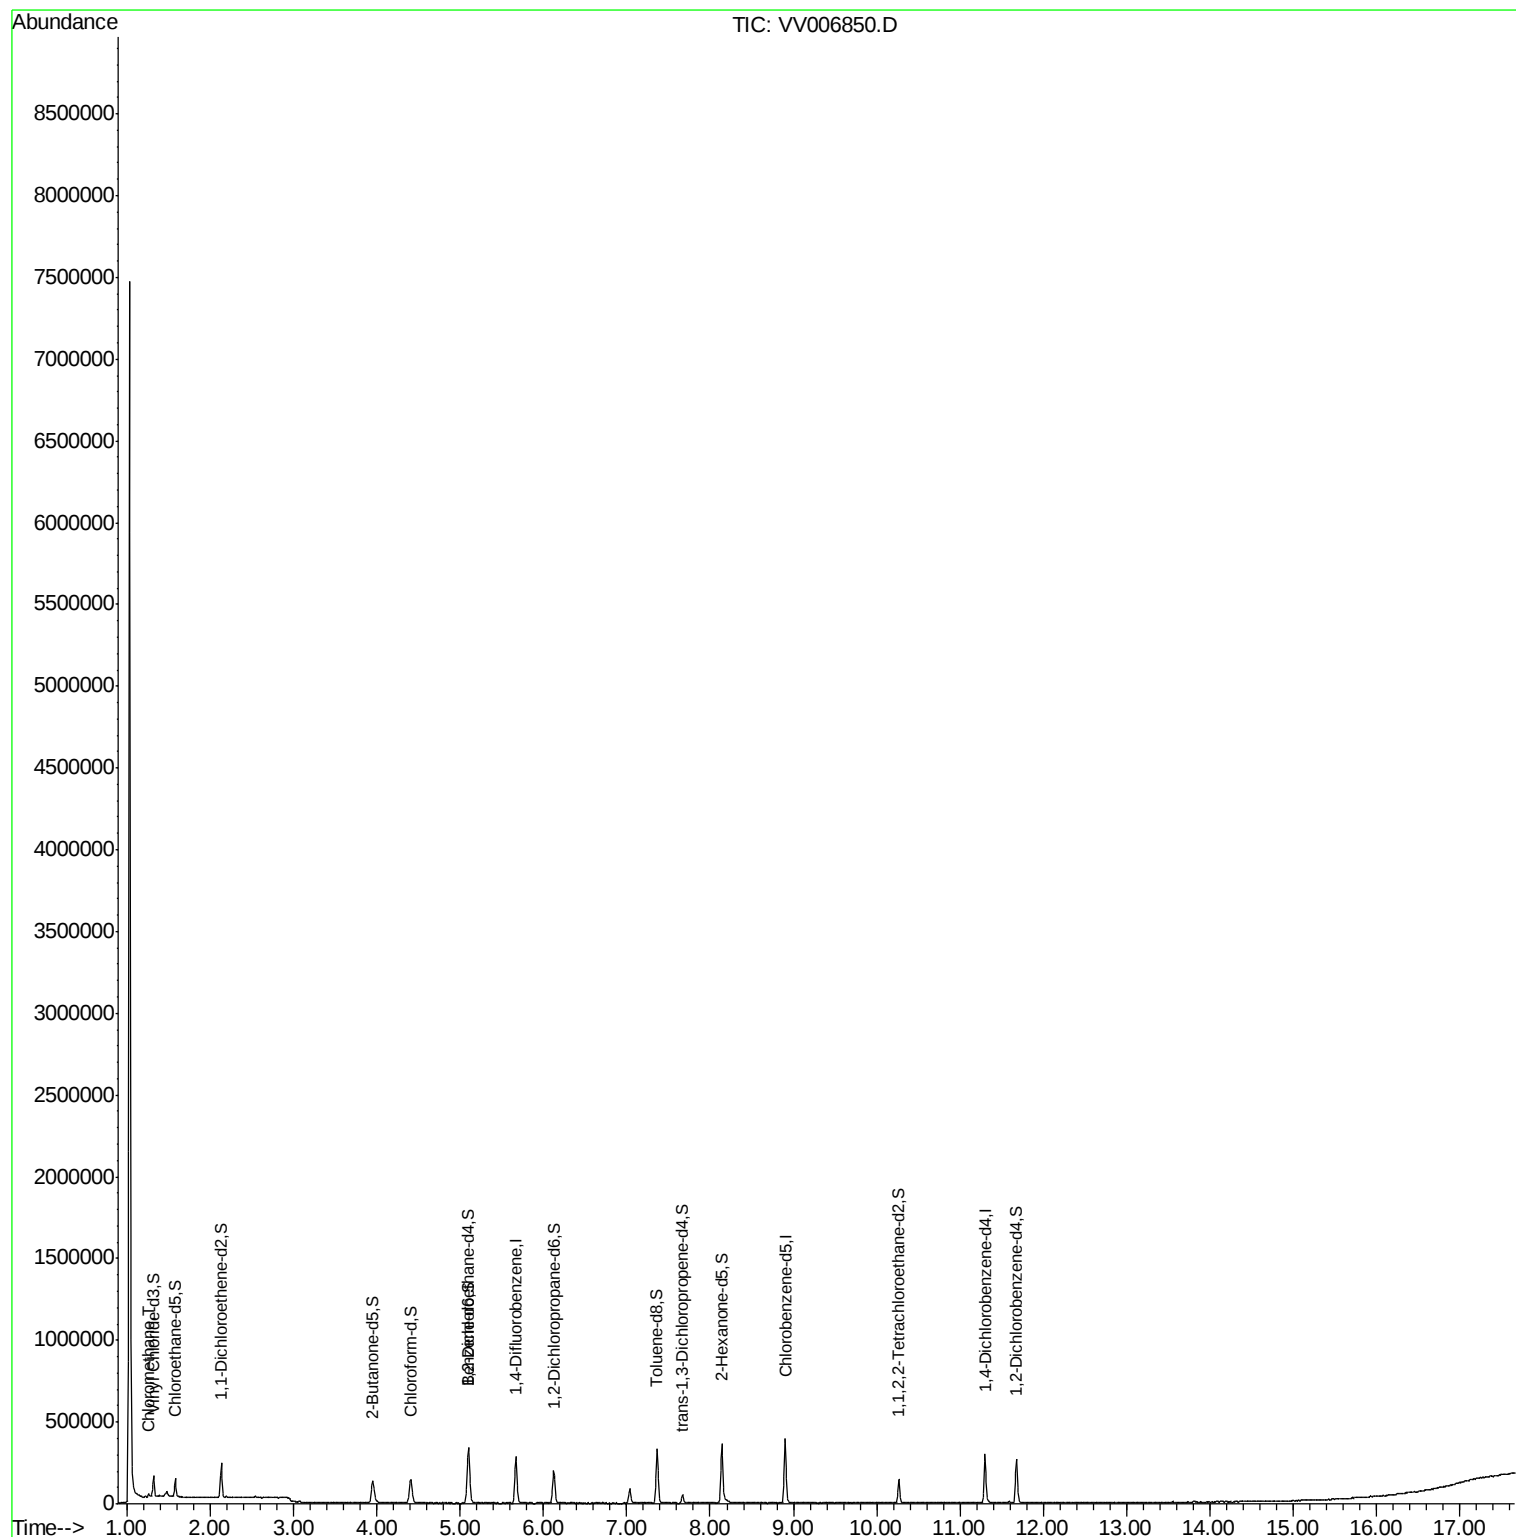

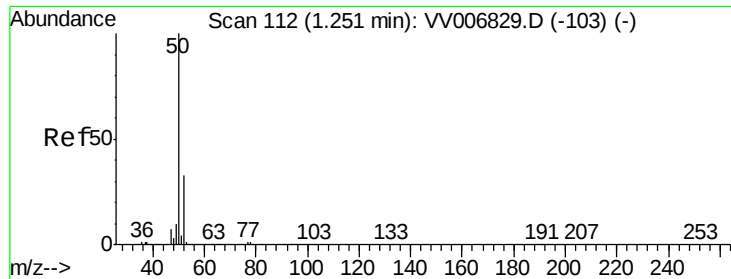

#3
 Chloromethane
 Concen: 0.63 ug/L
 RT: 1.25 min Scan# 113
 Delta R.T. 0.00 min
 Lab File: VV006850.D
 Acq: 03 Aug 2018 11:47

Instrument :
 MSVOA_V
 ClientSampleId :
 E5FA5

Tot Ion: 50 Resp: 17558
 Ion Ratio Lower Upper
 50 100
 52 31.9 23.3 43.3

