


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080218\
 Data File : VV006798.D
 Acq On : 02 Aug 2018 09:09
 Operator : SY/MD
 Sample : BFB75
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 03 04:21:42 2018

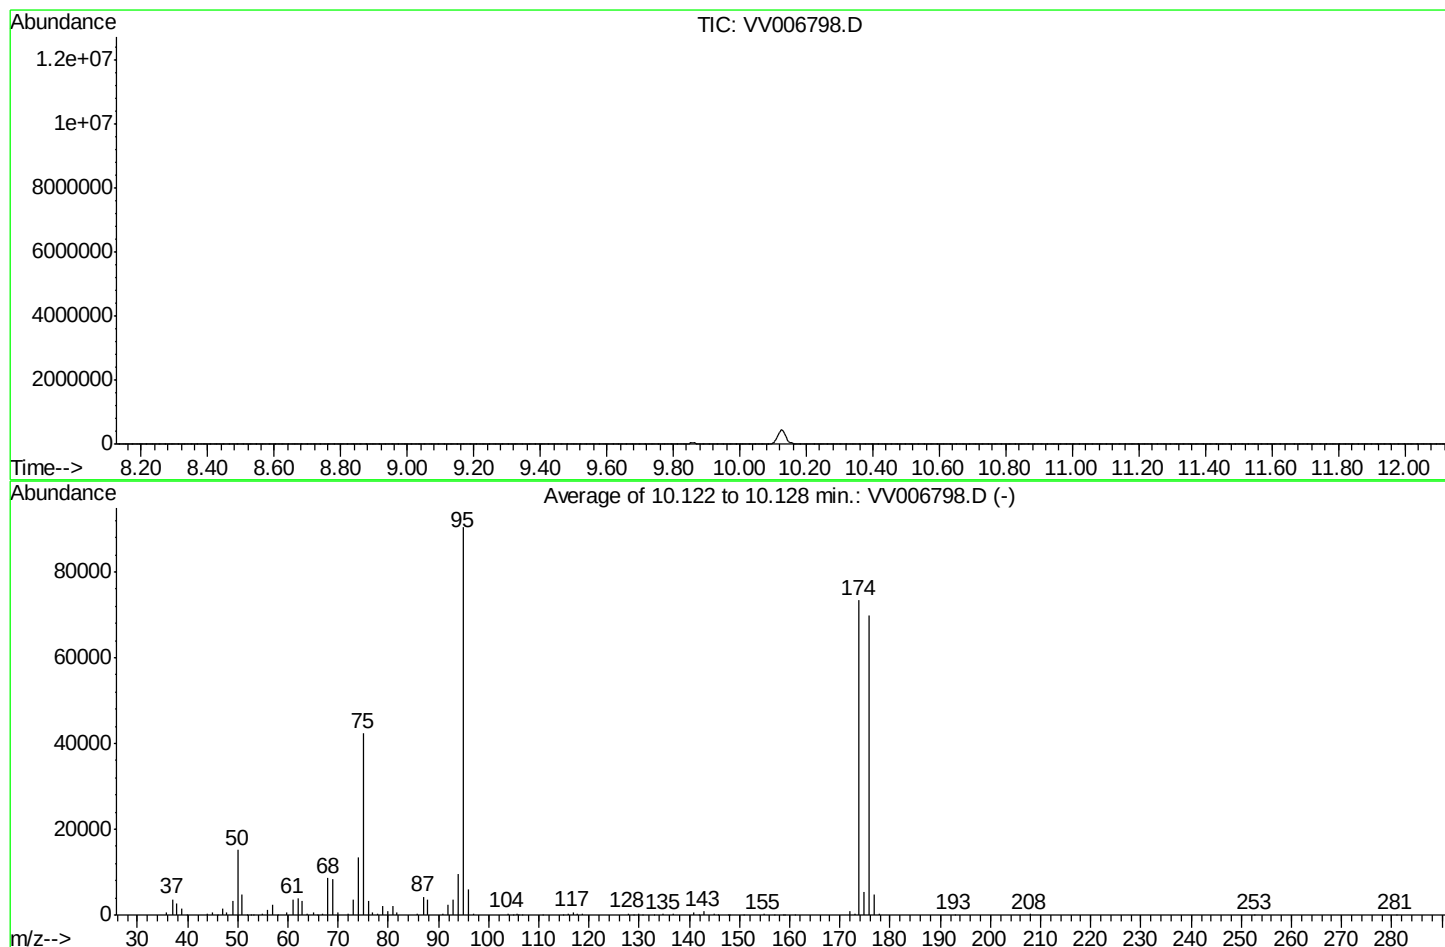

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	15225	PASS
75	95	30	80	46.7	42258	PASS
95	95	100	100	100.0	90416	PASS
96	95	5	9	6.5	5909	PASS
173	174	0.00	2	0.4	278	PASS
174	95	50	120	81.1	73338	PASS
175	174	5	9	7.5	5521	PASS
176	174	95	101	95.3	69874	PASS
177	176	5	9	6.9	4853	PASS

m/z	Abundance
35.80	308.0
38.00	245.0
38.90	124.0
39.90	605.0
40.90	184.0
41.80	223.0
43.00	229.0
43.80	1941.0
44.90	238.0
46.00	136.0
50.90	109.0
51.90	112.0
55.20	156.0
63.90	216.0
66.80	129.0
77.00	318.0
78.00	187.0
88.70	106.0
96.00	227.0
102.90	123.0
132.80	230.0
147.00	110.0
190.70	149.0
192.80	170.0
206.90	1542.0
207.90	235.0
209.00	280.0
269.00	287.0
280.80	197.0
282.00	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.80	889.0
36.90	3669.0
37.90	2917.0
38.90	1661.0
39.70	468.0
41.00	132.0
41.90	123.0
42.90	213.0
43.90	2107.0
44.90	686.0
46.00	168.0
46.90	1248.0
47.80	590.0
48.90	2967.0
49.90	15110.0
50.90	4918.0
51.80	223.0
52.70	122.0
54.90	303.0
55.80	1196.0
56.90	2316.0
58.10	107.0
59.80	684.0
60.90	3605.0
61.90	3577.0
62.90	3014.0
64.00	530.0
65.10	610.0
65.90	116.0
66.80	296.0
67.90	8195.0
68.90	8244.0
70.00	642.0
71.90	384.0
72.90	3118.0
73.90	13150.0
74.90	40720.0
76.00	3267.0
76.90	821.0
77.80	596.0
78.80	2094.0
79.80	750.0
80.80	1989.0
81.80	820.0
85.60	234.0
87.00	3965.0
87.90	3741.0
90.80	373.0
91.90	2218.0
92.90	3765.0
93.90	9008.0
94.90	87080.0
95.90	5937.0
97.10	239.0
103.70	249.0
104.80	121.0
105.70	345.0
106.70	117.0
110.80	156.0
114.80	154.0
115.80	239.0
116.80	610.0
117.70	356.0
118.70	371.0
127.70	289.0
128.90	138.0
129.70	278.0
130.70	133.0
132.90	352.0
134.70	279.0
136.80	205.0
140.80	720.0
142.80	732.0
144.90	187.0
145.80	145.0
147.70	104.0
154.80	185.0
156.90	103.0
171.80	882.0
173.00	835.0
173.80	69312.0
174.80	5194.0
175.80	65536.0
176.90	4456.0
177.70	201.0
190.70	106.0
192.80	166.0
206.90	1533.0
207.90	430.0
208.90	233.0
268.90	193.0
281.00	328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.80	849.0
36.90	3887.0
37.90	2991.0
38.90	1801.0
39.90	562.0
41.00	160.0
41.90	157.0
42.90	212.0
43.90	2100.0
44.80	796.0
45.90	196.0
46.90	1513.0
47.80	561.0
48.90	3373.0
49.90	15652.0
50.90	5176.0
51.80	222.0
52.70	131.0
55.00	349.0
55.80	1201.0
56.90	2560.0
58.00	167.0
59.80	713.0
61.00	3711.0
61.90	3842.0
62.90	3320.0
63.90	588.0
65.00	644.0
65.90	152.0
66.90	336.0
67.90	8846.0
68.90	8687.0
69.90	650.0
71.90	459.0
72.90	3641.0
73.90	13784.0
74.90	43624.0
76.00	3463.0
76.90	838.0
77.90	656.0
78.80	2150.0
79.80	860.0
80.80	2124.0
81.80	759.0
85.60	208.0
86.90	4291.0
87.90	3814.0
90.80	406.0
91.90	2598.0
92.90	3748.0
93.90	9898.0
94.90	93624.0
95.90	6227.0
97.10	244.0
103.80	322.0
104.80	165.0
105.70	304.0
106.70	116.0
110.80	159.0
114.80	121.0
115.90	272.0
116.80	651.0
117.70	319.0
118.70	371.0
127.70	309.0
128.90	146.0
129.80	283.0
130.70	114.0
132.90	378.0
134.80	302.0
136.80	181.0
140.80	728.0
141.90	133.0
142.80	895.0
144.90	194.0
145.70	133.0
148.00	167.0
154.80	202.0
156.80	121.0
158.70	106.0
160.90	118.0
171.90	881.0
173.90	75584.0
174.80	5764.0
175.80	71896.0
176.90	5058.0
177.70	162.0
190.60	129.0
192.90	208.0
206.90	1536.0
207.90	451.0
208.80	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

268.90177.0

281.00287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.80	856.0
36.90	3606.0
37.90	3034.0
38.90	1772.0
39.90	744.0
40.90	203.0
41.90	179.0
42.80	216.0
43.80	2178.0
44.80	854.0
45.80	190.0
46.90	1644.0
47.80	511.0
48.90	3354.0
49.90	14914.0
50.90	4822.0
51.90	191.0
52.70	134.0
53.10	106.0
55.00	296.0
55.80	1085.0
56.90	2396.0
58.00	173.0
59.80	695.0
61.00	3449.0
61.90	3822.0
62.90	3205.0
63.80	620.0
64.90	668.0
65.90	124.0
66.90	291.0
67.90	8732.0
68.90	8312.0
69.90	616.0
71.80	445.0
72.90	3647.0
73.90	13391.0
74.90	42432.0
76.00	3477.0
76.90	770.0
77.90	676.0
78.80	2024.0
79.80	851.0
80.80	2138.0
81.70	635.0
85.70	168.0
86.90	4296.0
87.80	3626.0
90.80	396.0
91.90	2600.0
92.90	3492.0
93.90	9921.0
94.90	90544.0
95.90	6246.0
97.00	227.0
102.80	113.0
103.80	416.0
104.80	165.0
105.90	275.0
110.90	125.0
115.80	283.0
116.80	609.0
117.80	299.0
118.70	376.0
127.80	323.0
128.70	132.0
129.80	249.0
133.00	371.0
134.80	303.0
136.90	168.0
140.80	617.0
141.80	133.0
142.80	891.0
144.90	199.0
147.90	215.0
150.80	102.0
154.70	179.0
156.80	165.0
159.00	112.0
160.90	139.0
171.90	943.0
173.80	75120.0
174.80	5606.0
175.80	72192.0
176.90	5045.0
177.80	187.0
190.60	175.0
192.90	197.0
206.90	1550.0
207.90	435.0
208.80	233.0
252.70	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

268.90	175.0
280.90	261.0
281.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75