
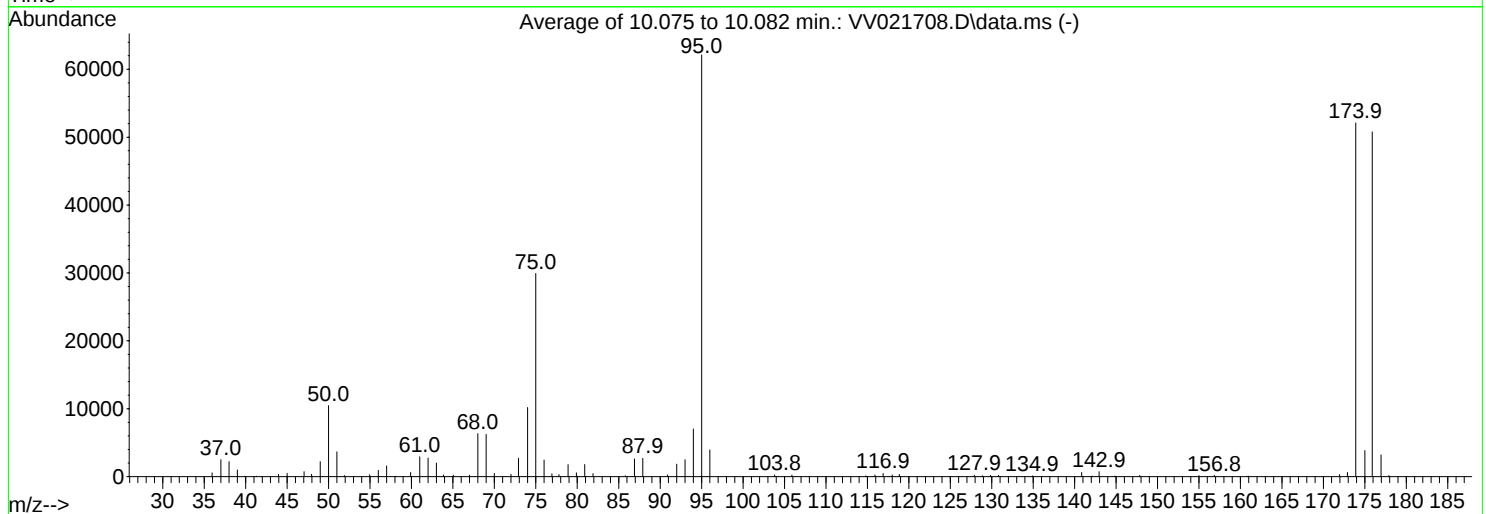


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080221\
 Data File : VV021708.D
 Acq On : 02 Aug 2021 08:53
 Operator : SY/MD
 Sample : BFB211
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB211

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 04 01:10:57 2021

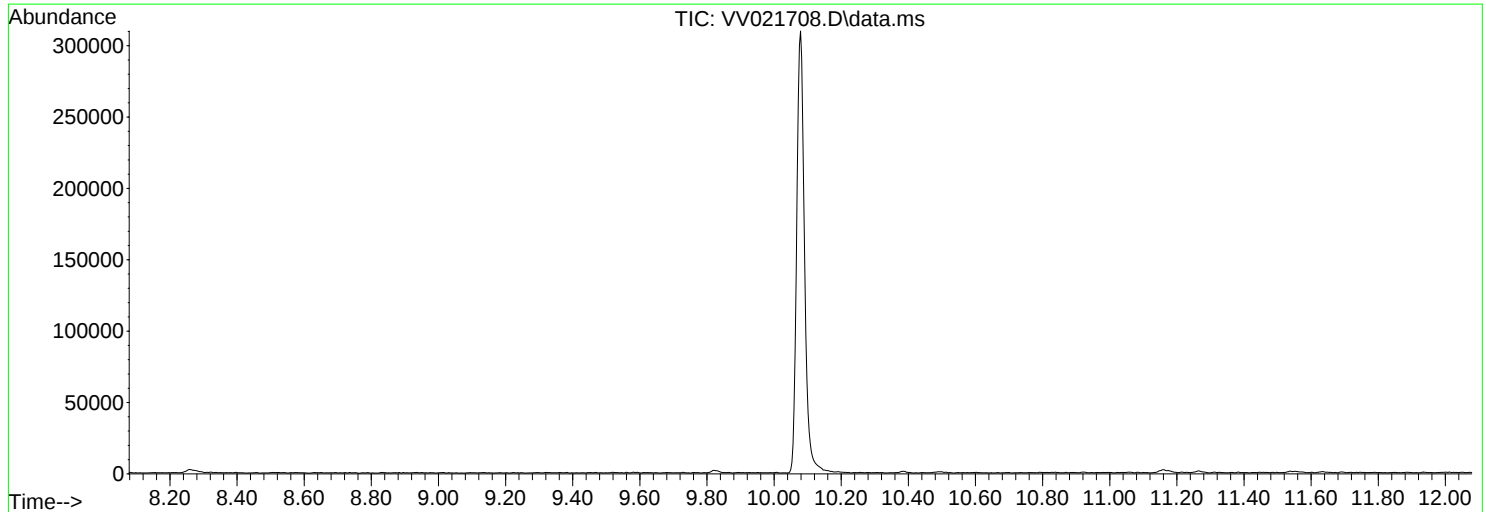

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10456	PASS
75	95	30	80	48.2	29928	PASS
95	95	100	100	100.0	62133	PASS
96	95	5	9	6.3	3944	PASS
173	174	0.00	2	1.2	624	PASS
174	95	50	120	83.9	52109	PASS
175	174	5	9	7.4	3837	PASS
176	174	95	105	97.5	50792	PASS
177	176	5	10	6.3	3214	PASS

Scan 2799 (10.040 min): VV021708.D\data.ms
BFB211

m/z	Abundance
40.00	230.0
44.00	500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	590.0
37.00	2609.0
38.00	2278.0
39.00	973.0
39.90	302.0
41.90	103.0
43.00	133.0
43.90	840.0
45.00	507.0
47.10	721.0
47.90	382.0
49.00	2304.0
50.00	10510.0
51.00	3693.0
51.90	163.0
55.00	314.0
56.00	936.0
57.00	1561.0
58.00	118.0
59.90	664.0
61.00	2766.0
62.00	2784.0
63.00	1986.0
63.90	238.0
65.00	189.0
67.00	228.0
68.00	6537.0
69.00	6311.0
70.00	435.0
72.00	381.0
72.90	2768.0
74.00	10021.0
75.00	30208.0
76.00	2522.0
77.00	371.0
77.80	315.0
78.90	1889.0
79.90	599.0
80.90	1795.0
81.90	414.0
85.80	167.0
86.90	2562.0
87.90	2701.0
90.90	286.0
92.00	1868.0
93.00	2542.0
94.00	7090.0
95.00	62248.0
96.00	4087.0
103.80	240.0
105.90	246.0
114.80	119.0
115.90	234.0
116.90	464.0
118.00	313.0
118.80	314.0
127.90	198.0
128.90	161.0
129.90	167.0
130.80	167.0
134.90	110.0
140.80	618.0
143.00	625.0
147.80	210.0
155.00	195.0
156.90	175.0
160.80	120.0
172.00	366.0
172.90	573.0
173.90	51032.0
175.00	3848.0
175.90	50344.0
177.00	3347.0
177.80	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	587.0
37.00	2573.0
38.00	2251.0
39.00	1030.0
39.90	291.0
41.30	104.0
44.00	824.0
45.00	510.0
47.10	705.0
47.90	369.0
49.00	2333.0
50.00	10731.0
51.00	3763.0
51.90	171.0
54.90	270.0
56.00	980.0
57.00	1615.0
58.10	102.0
59.90	637.0
61.00	3057.0
62.00	2861.0
63.00	2056.0
63.90	248.0
65.10	194.0
67.00	247.0
68.00	6517.0
69.00	6412.0
70.00	492.0
72.00	353.0
72.90	2867.0
74.00	10570.0
75.00	30800.0
76.00	2508.0
76.90	426.0
77.80	332.0
78.90	1823.0
79.90	572.0
80.90	1850.0
81.90	464.0
85.80	161.0
86.90	2793.0
87.90	2711.0
90.90	278.0
92.00	1896.0
93.00	2558.0
94.00	7236.0
95.00	64280.0
96.00	3988.0
103.80	282.0
105.90	255.0
114.80	139.0
115.90	258.0
116.90	481.0
118.00	296.0
118.90	345.0
127.90	209.0
128.80	153.0
129.80	203.0
130.80	204.0
134.90	137.0
140.80	641.0
142.10	113.0
143.00	743.0
144.90	118.0
147.80	199.0
155.00	166.0
156.90	185.0
161.00	113.0
172.00	310.0
172.90	638.0
173.90	53904.0
175.00	4001.0
175.90	52376.0
177.00	3277.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
35.90	498.0
37.00	2315.0
38.00	2129.0
39.00	982.0
39.90	287.0
41.30	132.0
44.00	829.0
45.00	466.0
46.90	746.0
48.00	330.0
49.00	2039.0
50.00	10126.0
51.00	3507.0
51.90	171.0
54.90	248.0
56.00	845.0
57.00	1575.0
59.90	518.0
61.00	2919.0
62.00	2542.0
63.00	1988.0
63.80	242.0
65.10	222.0
67.00	200.0
68.00	5971.0
69.00	5927.0
70.00	492.0
72.00	345.0
72.90	2521.0
74.00	9983.0
75.00	28776.0
76.00	2326.0
76.90	484.0
77.80	311.0
78.90	1631.0
79.90	508.0
80.90	1745.0
81.90	466.0
85.80	124.0
86.90	2513.0
87.90	2672.0
90.90	236.0
92.00	1735.0
93.00	2366.0
94.00	6774.0
95.00	59872.0
96.00	3756.0
103.80	282.0
105.90	240.0
114.80	114.0
115.90	266.0
116.90	498.0
118.00	205.0
118.90	342.0
127.90	198.0
128.80	141.0
129.80	221.0
130.80	177.0
134.90	115.0
140.90	615.0
142.10	145.0
142.90	795.0
144.80	135.0
147.90	174.0
155.00	143.0
156.80	185.0
161.00	103.0
171.90	261.0
172.90	661.0
173.90	51392.0
175.00	3663.0
175.90	49656.0
176.90	3018.0
178.00	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211