

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006855.D
 Acq On : 03 Aug 2018 19:49
 Operator : SY/MD
 Sample : J4204-22
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Aug 04 04:47:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 04 04:38:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	223058	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	203565	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	79751	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	92806	6.01	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	120.20%
7) Chloroethane-d5	1.58	69	80758	6.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.20%
11) 1,1-Dichloroethene-d2	2.13	63	129278	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.20%
20) 2-Butanone-d5	3.98	46	236848	63.21	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.42%
24) Chloroform-d	4.41	84	157356	5.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.40%
26) 1,2-Dichloroethane-d4	5.09	65	84208	6.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.60%
32) Benzene-d6	5.10	84	302670	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.20%
36) 1,2-Dichloropropane-d6	6.12	67	105575	5.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.40%
41) Toluene-d8	7.37	98	235588	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
43) trans-1,3-Dichloropropene-	7.67	79	34415	5.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.20%
46) 2-Hexanone-d5	8.15	63	149915	52.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.94%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	84471	6.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.20%#
64) 1,2-Dichlorobenzene-d4	11.68	152	81912	5.54	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	10690	4.05 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080318\
Data File : VV006855.D
Acq On : 03 Aug 2018 19:49
Operator : SY/MD
Sample : J4204-22
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Aug 04 04:47:03 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 04 04:38:24 2018
Response via : Initial Calibration

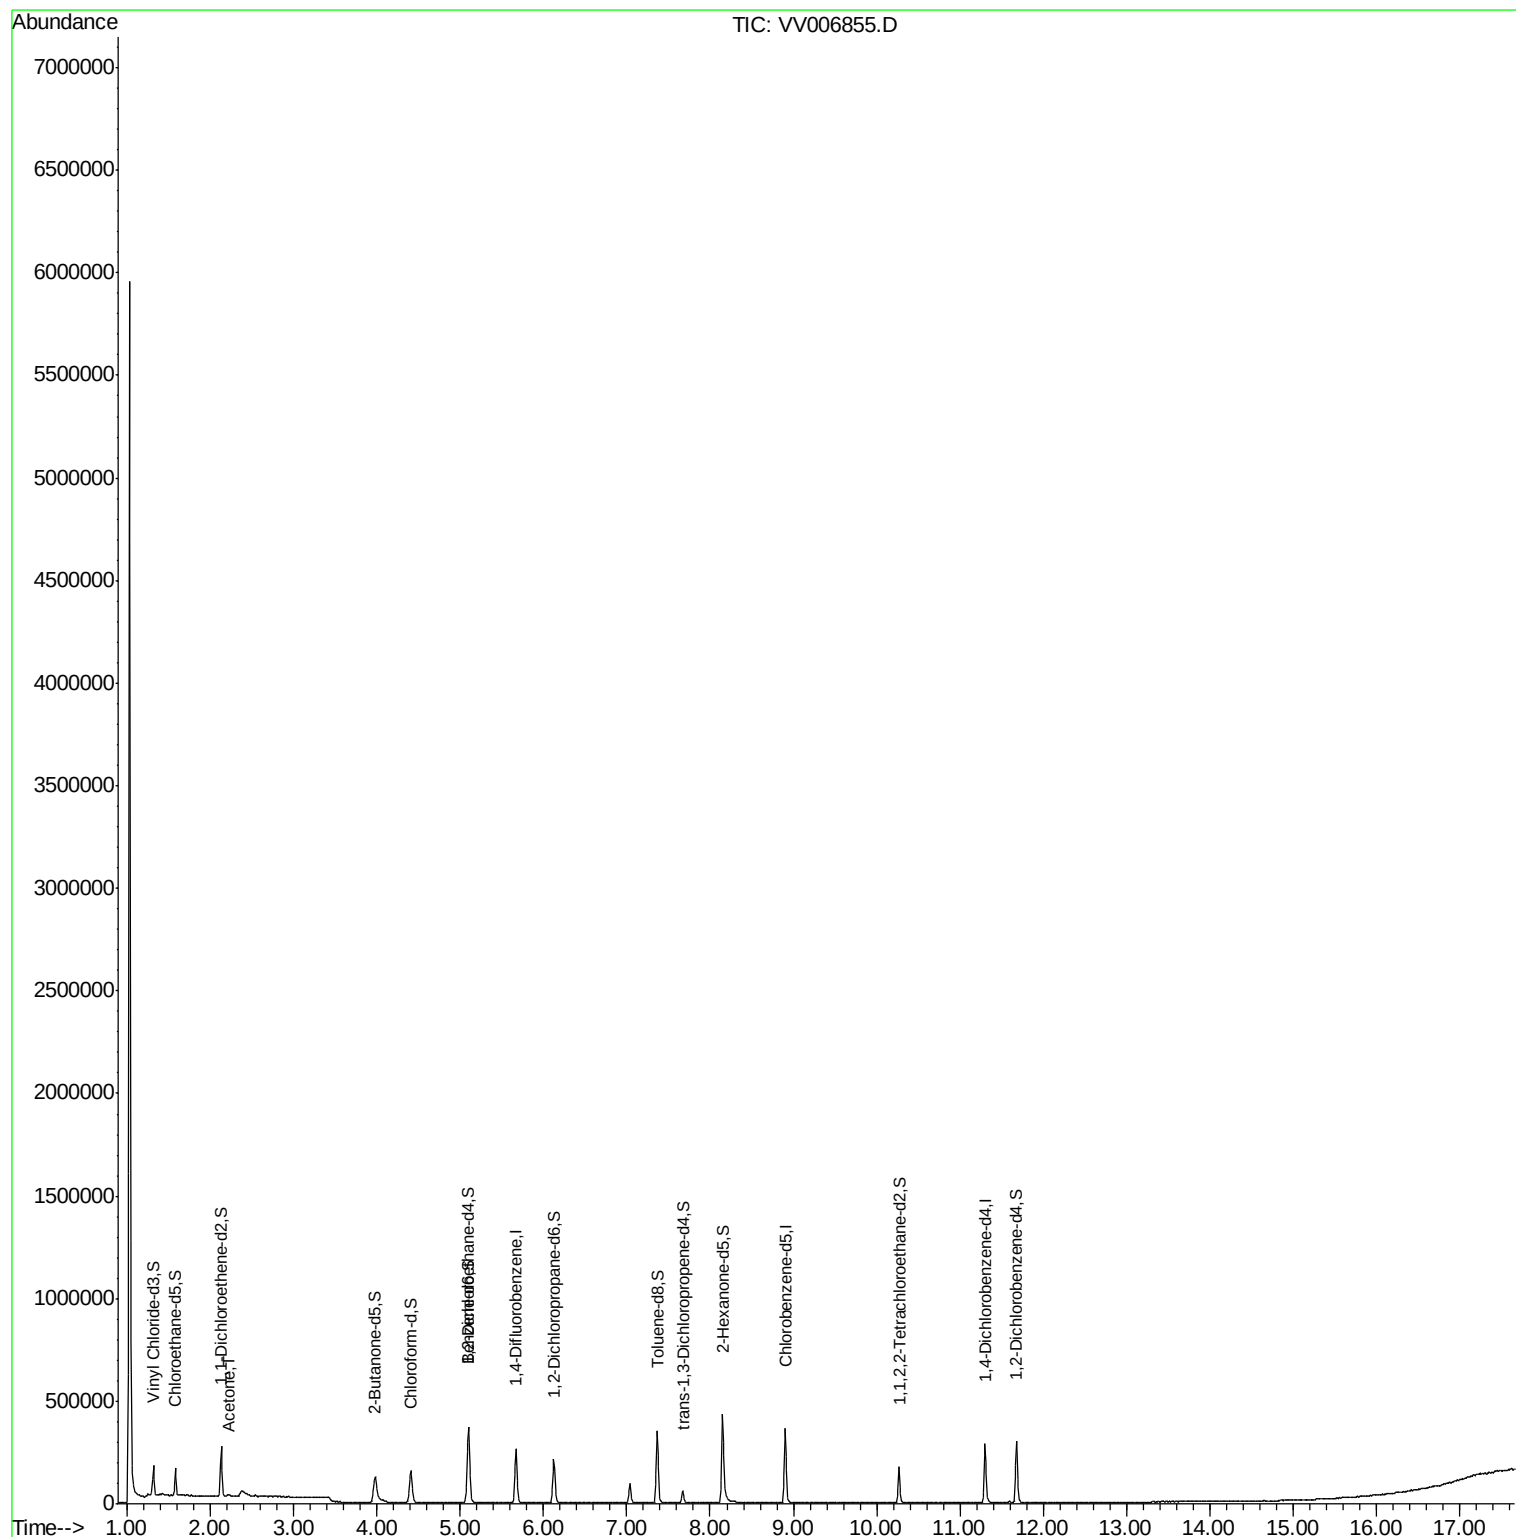

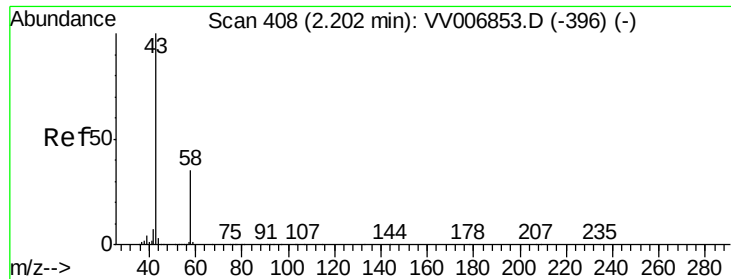

#13

Acetone

Concen: 4.05 ug/L

RT: 2.21 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV006855.D

Acq: 03 Aug 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :

VHBLK02

Tot Ion: 43 Resp: 10690

Ion Ratio Lower Upper

43 100

58 42.4 0.0 69.0

