

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006856.D
 Acq On : 03 Aug 2018 20:15
 Operator : SY/MD
 Sample : J4261-22
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Aug 04 04:51:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 04 04:38:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	223402	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	210781	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	81753	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	90153	5.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.60%
7) Chloroethane-d5	1.58	69	80256	5.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.40%
11) 1,1-Dichloroethene-d2	2.13	63	128492	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.60%
20) 2-Butanone-d5	3.98	46	236833	63.11	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.22%
24) Chloroform-d	4.41	84	154994	5.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.40%
26) 1,2-Dichloroethane-d4	5.09	65	82986	6.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.60%
32) Benzene-d6	5.10	84	301471	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
36) 1,2-Dichloropropane-d6	6.12	67	102490	5.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.20%
41) Toluene-d8	7.37	98	232139	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.67	79	32152	4.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.80%
46) 2-Hexanone-d5	8.15	63	149083	50.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.78%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	82105	5.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	117.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	81295	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	19245	7.27 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080318\
Data File : VV006856.D
Acq On : 03 Aug 2018 20:15
Operator : SY/MD
Sample : J4261-22
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Aug 04 04:51:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 04 04:38:24 2018
Response via : Initial Calibration

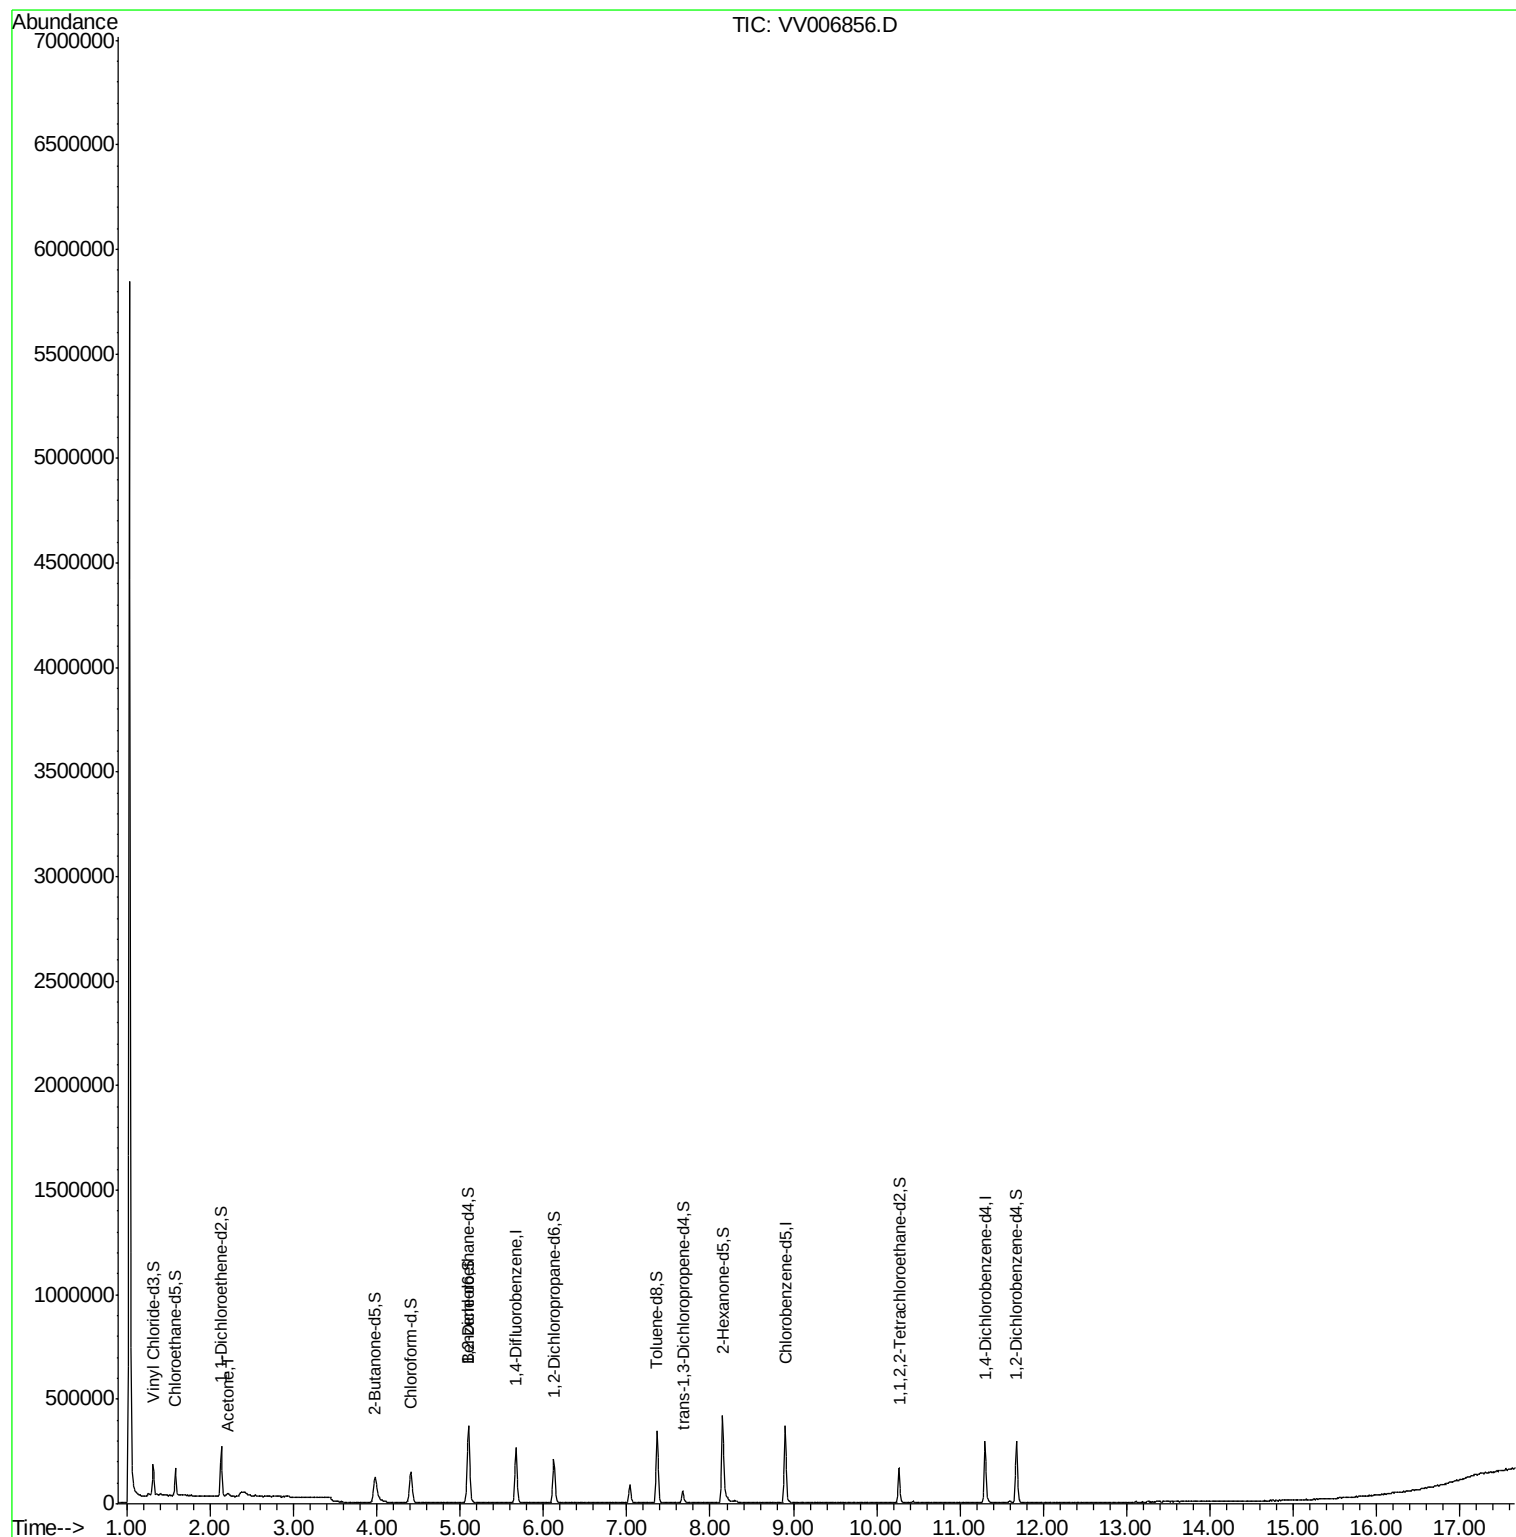

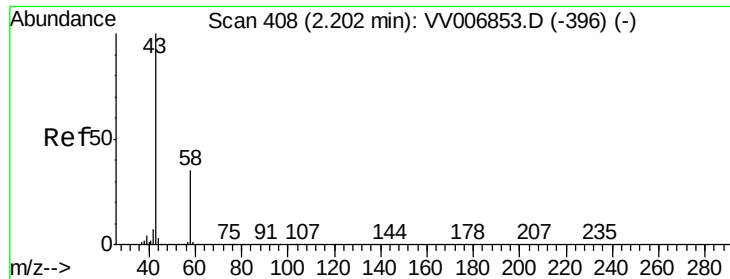

#13

Acetone

Concen: 7.27 ug/L

RT: 2.21 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV006856.D

Acq: 03 Aug 2018 20:15

Instrument :

MSVOA_V

ClientSampleId :

VHBLK02

Tot Ion: 43 Resp: 19245

Ion Ratio Lower Upper

43 100

58 30.3 0.0 69.0

