

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006857.D
 Acq On : 03 Aug 2018 20:42
 Operator : SY/MD
 Sample : J4225-23
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Aug 04 04:56:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 04 04:38:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	87535	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	82591	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	33147	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	94936	15.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	313.20%#
7) Chloroethane-d5	1.58	69	84398	16.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	320.20%#
11) 1,1-Dichloroethene-d2	2.13	63	131655	11.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	234.20%#
20) 2-Butanone-d5	3.98	46	243656	165.71	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	331.42%#
24) Chloroform-d	4.41	84	163396	15.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	308.00%#
26) 1,2-Dichloroethane-d4	5.09	65	89113	16.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	333.00%#
32) Benzene-d6	5.10	84	312582	14.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	280.20%#
36) 1,2-Dichloropropane-d6	6.12	67	109151	14.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	296.60%#
41) Toluene-d8	7.37	98	240639	12.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	241.80%#
43) trans-1,3-Dichloropropene-	7.67	79	35743	13.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	274.60%#
46) 2-Hexanone-d5	8.15	63	154811	133.54	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	267.08%#
57) 1,1,2,2-Tetrachloroethane-	10.27	84	87790	16.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	320.40%#
64) 1,2-Dichlorobenzene-d4	11.68	152	83199	13.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	270.60%#


Target Compounds					Ovalue
13) Acetone	2.22	43	14791	14.26 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
Data File : VV006857.D
Acq On : 03 Aug 2018 20:42
Operator : SY/MD
Sample : J4225-23
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Aug 04 04:56:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 04 04:38:24 2018
Response via : Initial Calibration

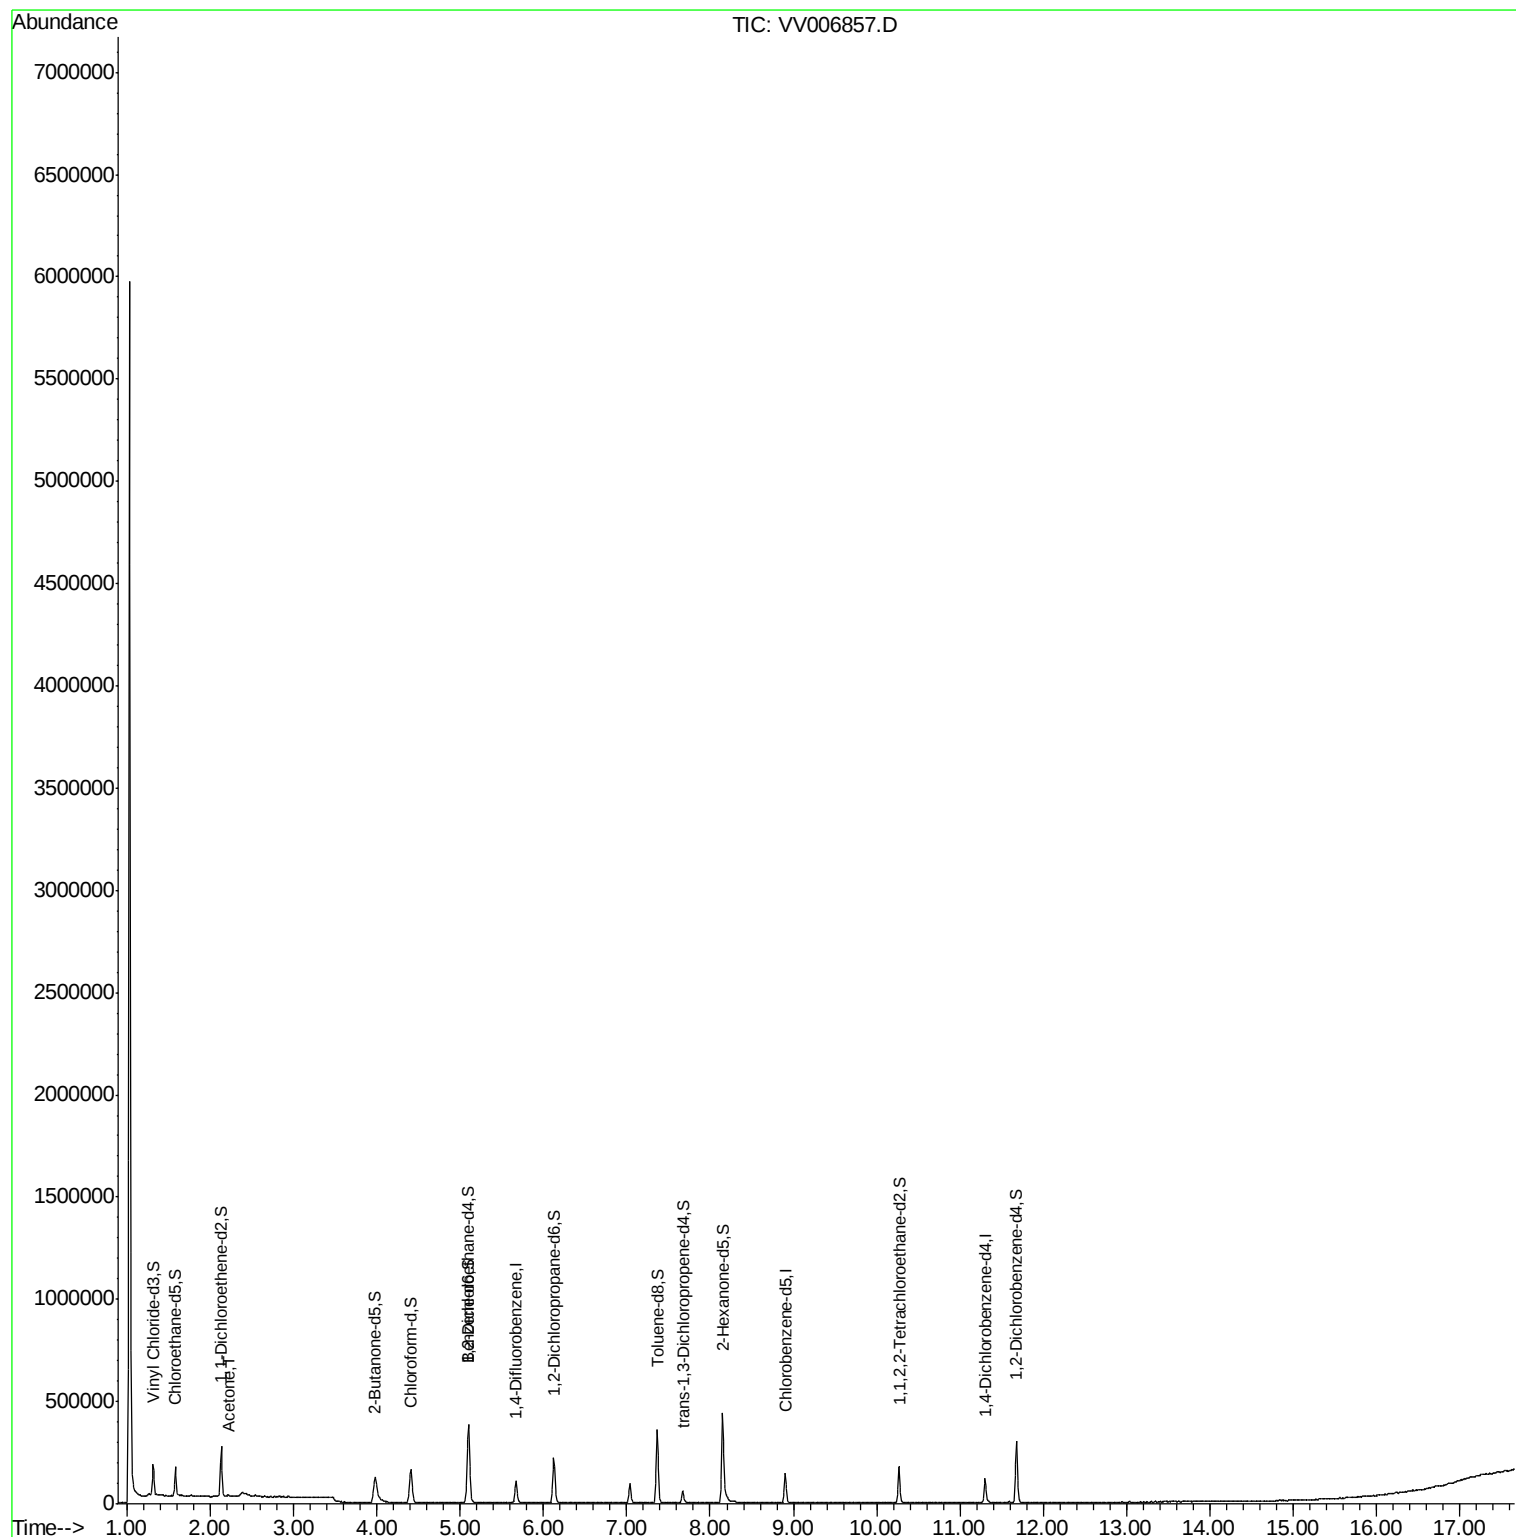

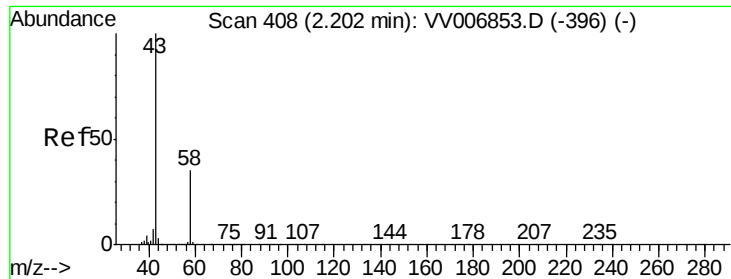

#13

Acetone

Concen: 14.26 ug/L

RT: 2.22 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV006857.D

Acq: 03 Aug 2018 20:42

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 14791

Ion Ratio Lower Upper

43 100

58 39.9 0.0 69.0

