

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006865.D
 Acq On : 04 Aug 2018 00:16
 Operator : SY/MD
 Sample : J4314-11
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KW9

Quant Time: Aug 04 05:49:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 04 04:38:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	217786	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	201800	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	78727	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	95877	6.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.20%
7) Chloroethane-d5	1.58	69	86092	6.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	131.20%#
11) 1,1-Dichloroethene-d2	2.13	63	136570	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.60%
20) 2-Butanone-d5	3.97	46	250540	68.48	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	136.96%#
24) Chloroform-d	4.41	84	171754	6.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	130.20%#
26) 1,2-Dichloroethane-d4	5.09	65	89125	6.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	133.80%#
32) Benzene-d6	5.10	84	319233	5.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.20%
36) 1,2-Dichloropropane-d6	6.12	67	110965	6.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	123.40%
41) Toluene-d8	7.37	98	241685	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
43) trans-1,3-Dichloropropene-	7.67	79	34556	5.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	108.60%
46) 2-Hexanone-d5	8.15	63	149473	52.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.54%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	86972	6.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	130.00%#
64) 1,2-Dichlorobenzene-d4	11.68	152	86959	5.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	7331	2.84 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
Data File : VV006865.D
Acq On : 04 Aug 2018 00:16
Operator : SY/MD
Sample : J4314-11
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KW9

Quant Time: Aug 04 05:49:45 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 04 04:38:24 2018
Response via : Initial Calibration

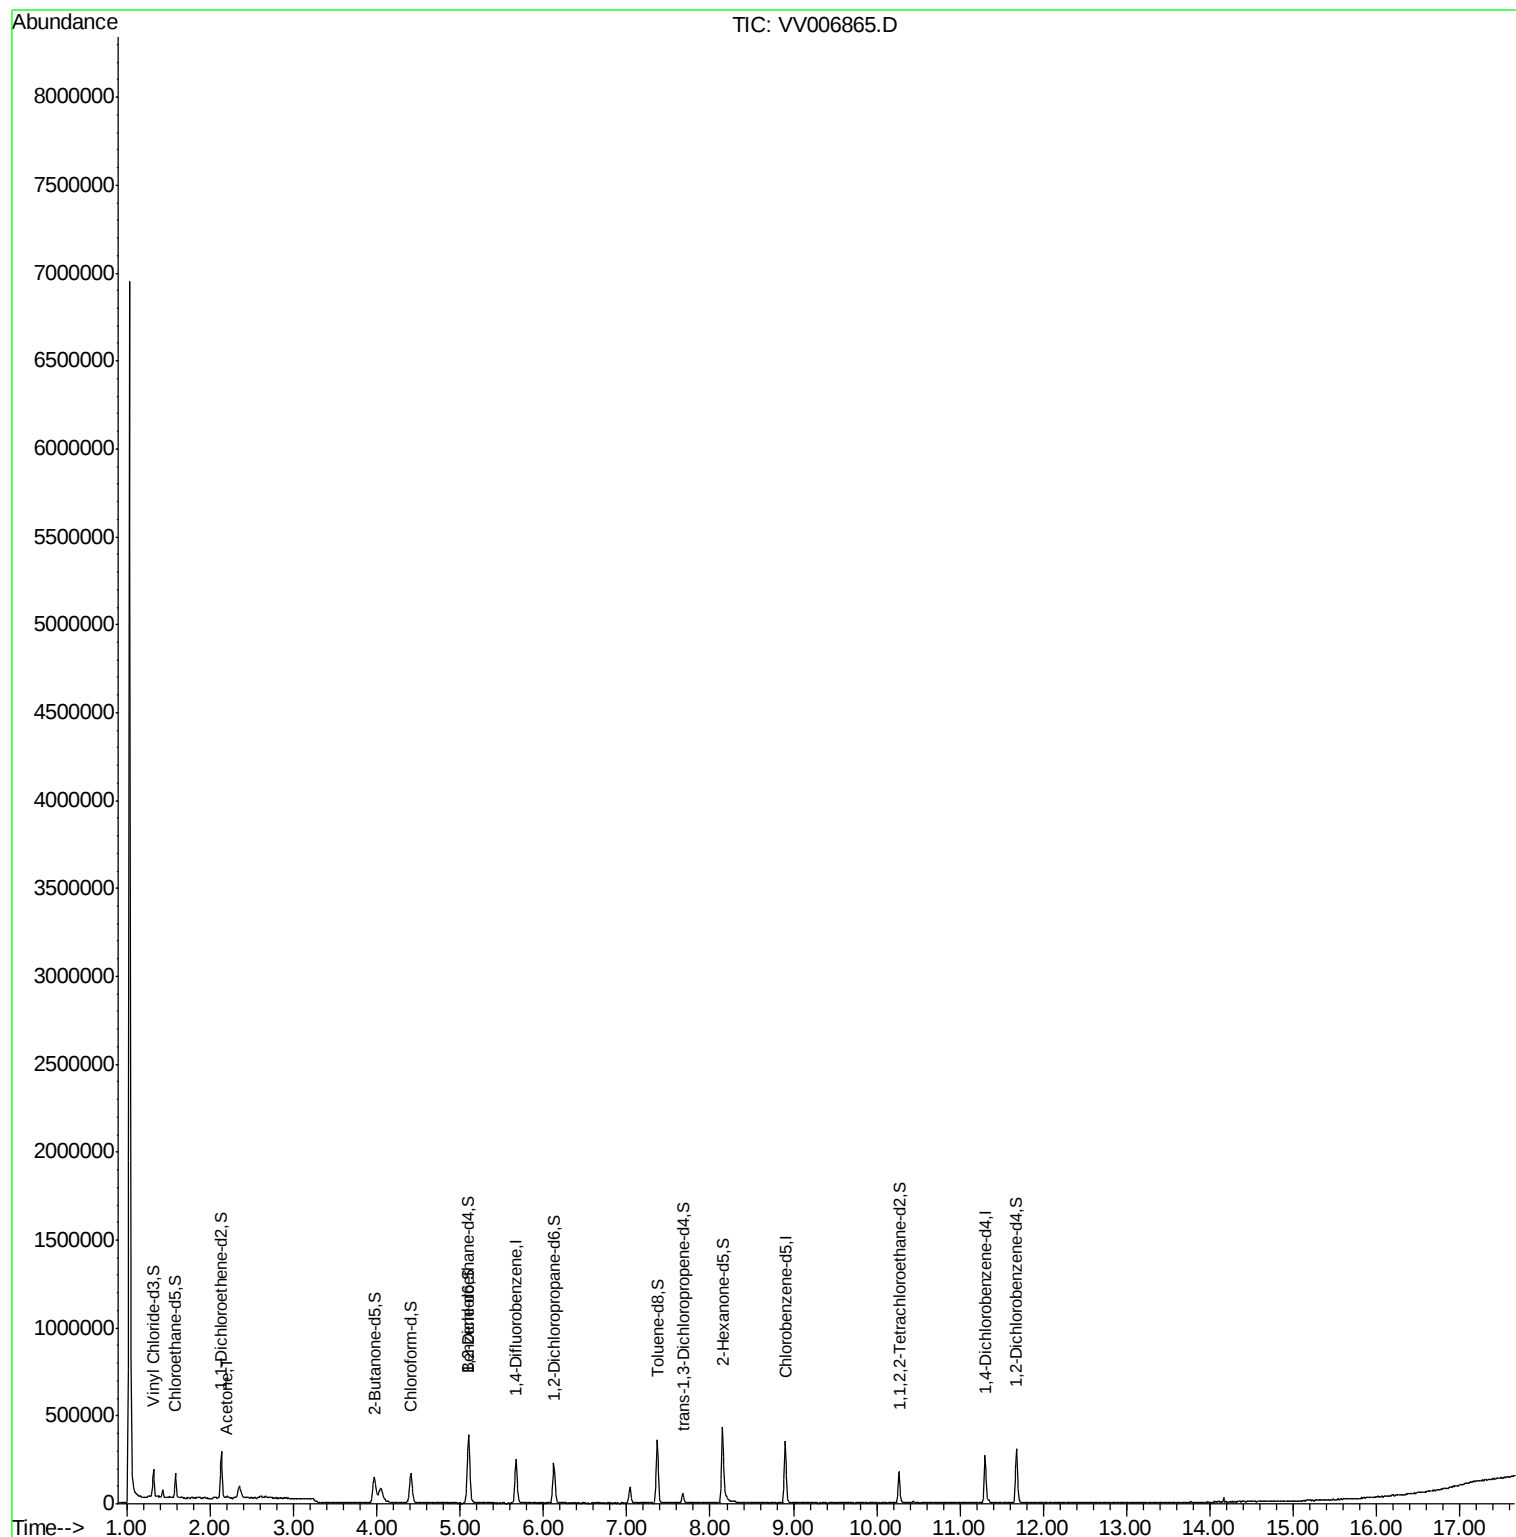

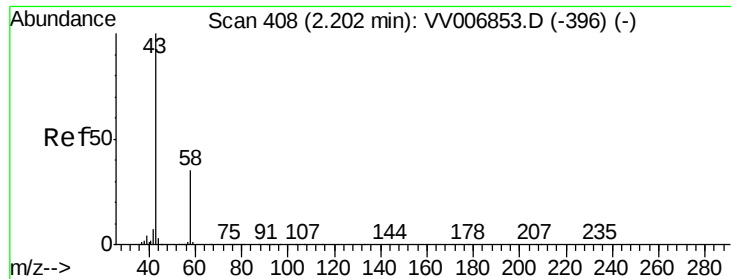

#13

Acetone

Concen: 2.84 ug/L

RT: 2.20 min Scan# 408

Delta R.T. -0.00 min

Lab File: VV006865.D

Acq: 04 Aug 2018 00:16

Instrument :

MSVOA_V

ClientSampleId :

C0KW9

Tot Ion: 43 Resp: 7331

Ion Ratio Lower Upper

43 100

58 40.4 0.0 69.0

