

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006869.D
 Acq On : 04 Aug 2018 02:03
 Operator : SY/MD
 Sample : J4314-15
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KX3

Quant Time: Aug 04 06:51:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 04 04:38:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	222784	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	211841	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	82463	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98289	6.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.40%
7) Chloroethane-d5	1.58	69	87428	6.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	130.40%#
11) 1,1-Dichloroethene-d2	2.13	63	137592	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.20%
20) 2-Butanone-d5	3.96	46	245654	65.64	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.28%#
24) Chloroform-d	4.41	84	173332	6.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	128.40%#
26) 1,2-Dichloroethane-d4	5.09	65	91951	6.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	135.00%#
32) Benzene-d6	5.10	84	328827	5.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.00%
36) 1,2-Dichloropropane-d6	6.12	67	110459	5.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	117.00%
41) Toluene-d8	7.37	98	248662	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	7.67	79	33027	4.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.80%
46) 2-Hexanone-d5	8.14	63	146953	49.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.84%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	88242	6.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.60%#
64) 1,2-Dichlorobenzene-d4	11.68	152	86184	5.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	7675	2.91 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080318\
Data File : VV006869.D
Acq On : 04 Aug 2018 02:03
Operator : SY/MD
Sample : J4314-15
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KX3

Quant Time: Aug 04 06:51:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 04 04:38:24 2018
Response via : Initial Calibration

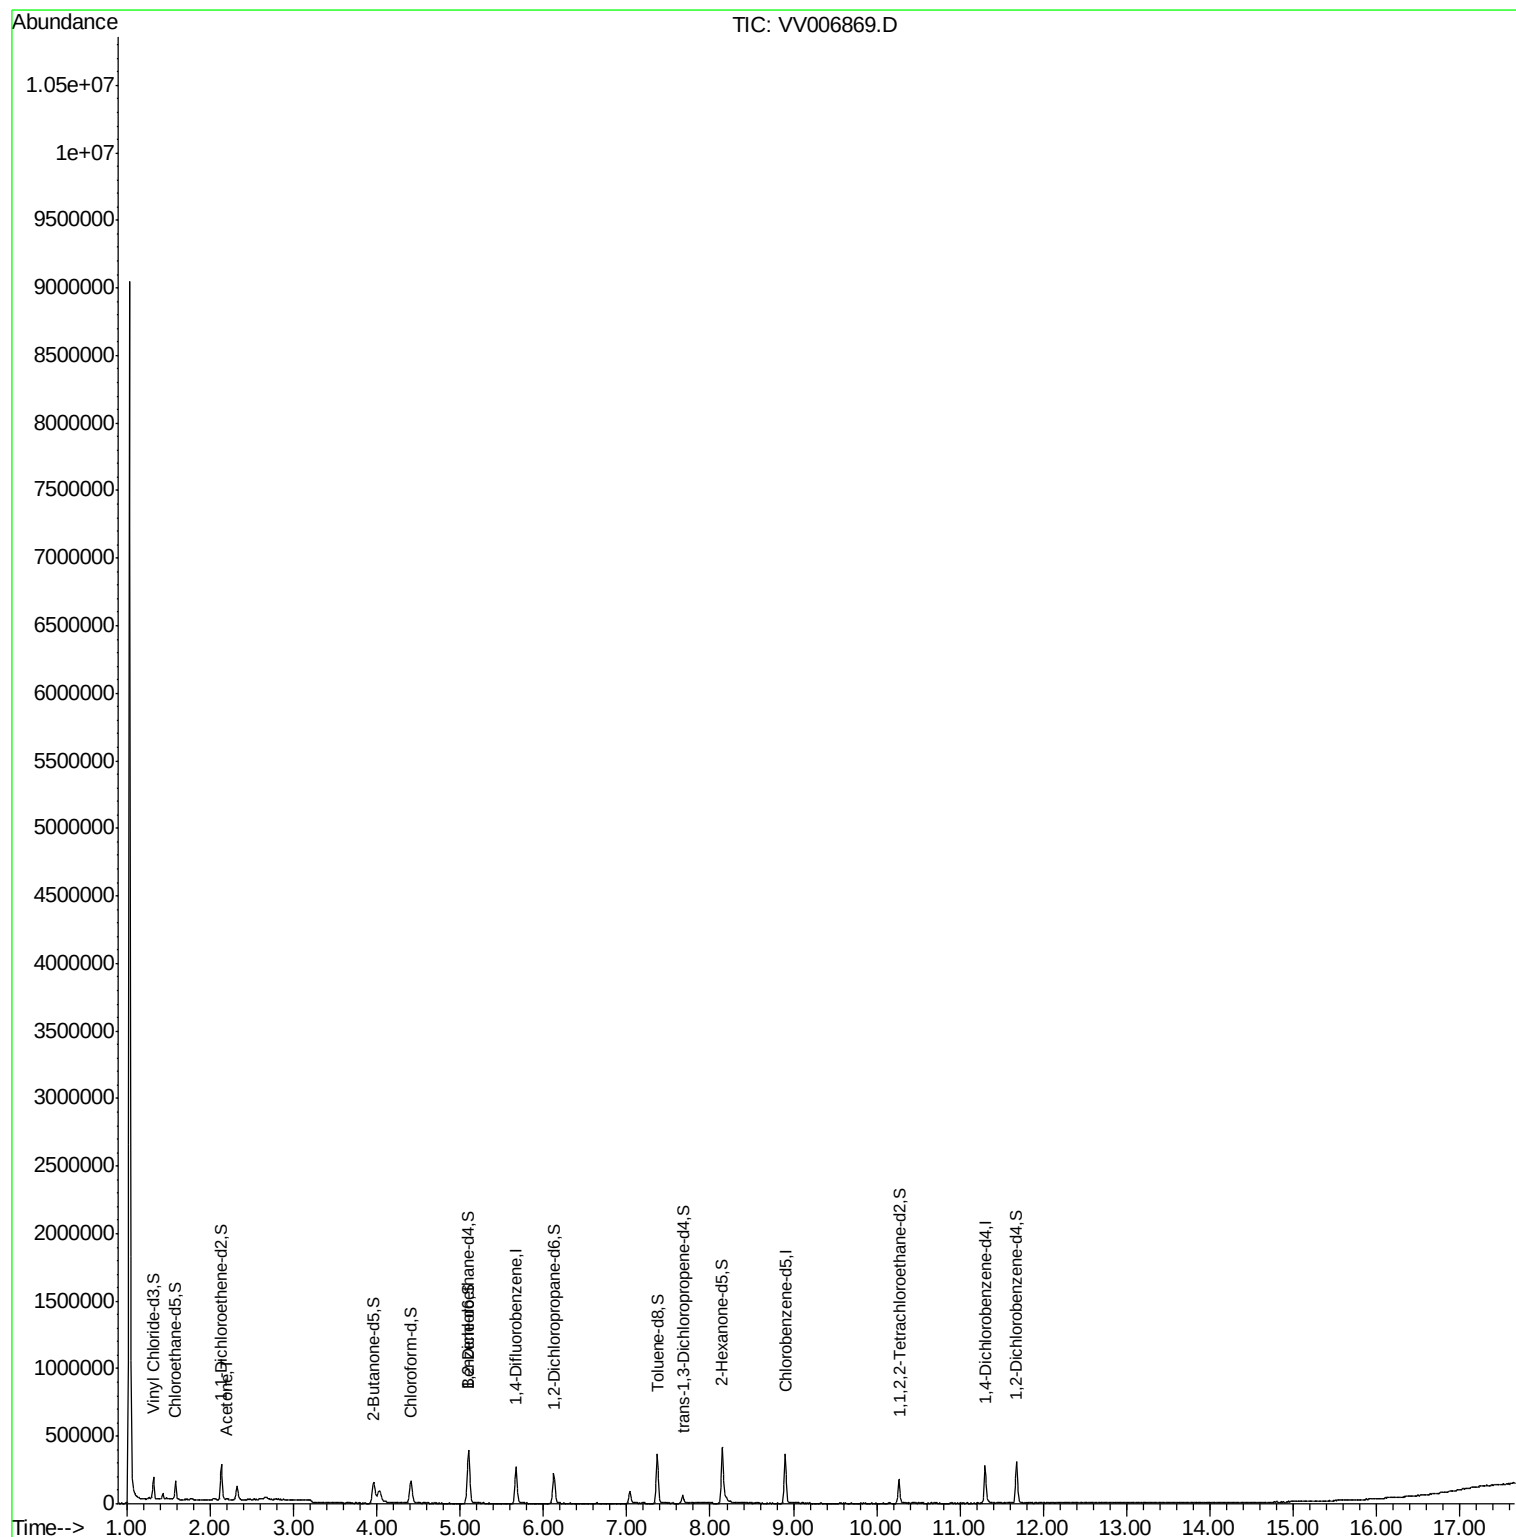

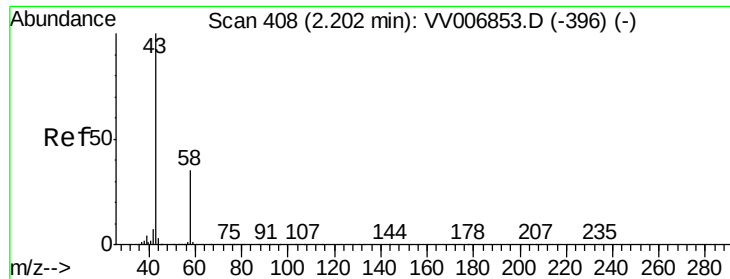

#13

Acetone

Concen: 2.91 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.01 min

Lab File: VV006869.D

Acq: 04 Aug 2018 02:03

Instrument :

MSVOA_V

ClientSampleId :

C0KX3

Tot Ion: 43 Resp: 7675

Ion Ratio Lower Upper

43 100

58 35.0 0.0 69.0

