


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080318\
 Data File : VV006852.D
 Acq On : 03 Aug 2018 15:12
 Operator : SY/MD
 Sample : BFB76
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 06 03:23:10 2018

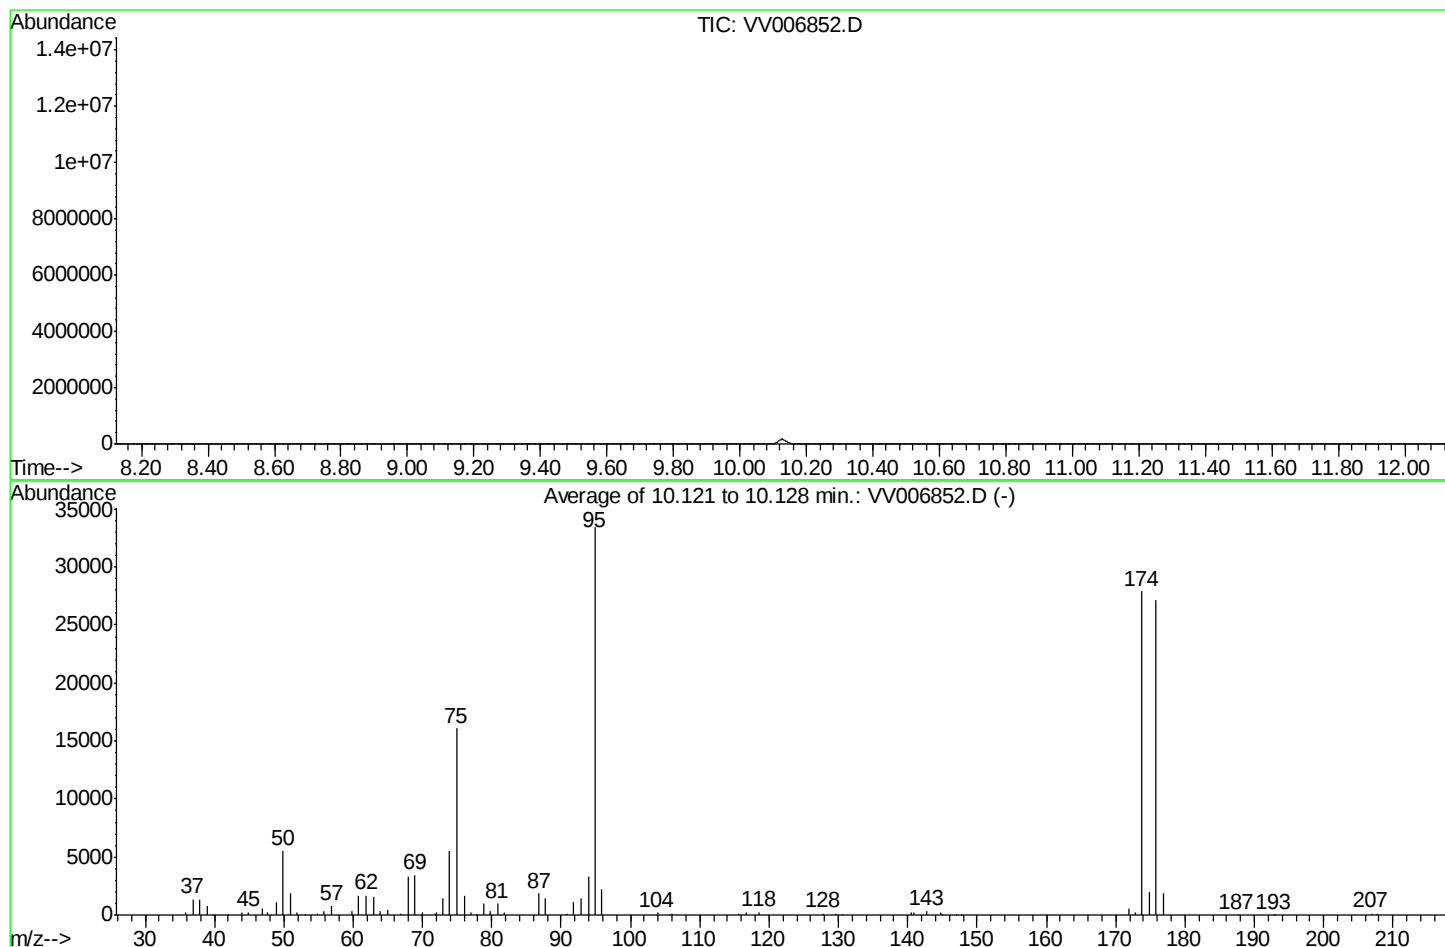

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5553	PASS
75	95	30	80	48.2	16100	PASS
95	95	100	100	100.0	33416	PASS
96	95	5	9	6.5	2168	PASS
173	174	0.00	2	0.8	217	PASS
174	95	50	120	83.5	27914	PASS
175	174	5	9	7.0	1958	PASS
176	174	95	101	97.1	27106	PASS
177	176	5	9	7.1	1919	PASS

Scan 2860 (10.086 min): VV006852.D
BFB76

m/z	Abundance
35.90	183.0
39.80	633.0
41.00	214.0
43.00	186.0
43.80	1648.0
45.00	133.0
72.90	105.0
76.90	164.0
77.70	180.0
95.70	106.0
206.90	644.0
208.00	196.0
208.70	140.0
252.80	114.0
269.00	268.0
281.00	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	385.0
36.90	1243.0
37.80	1327.0
39.00	770.0
39.70	628.0
40.80	152.0
42.80	178.0
43.90	1866.0
44.90	374.0
46.90	481.0
47.70	241.0
49.00	927.0
49.90	5504.0
50.90	1853.0
51.80	175.0
54.90	133.0
55.80	402.0
57.00	799.0
59.70	271.0
60.80	1526.0
61.90	1655.0
62.90	1519.0
63.80	282.0
65.00	494.0
66.70	133.0
67.90	3077.0
68.90	3171.0
69.90	261.0
71.80	190.0
72.90	1573.0
73.90	5306.0
74.90	15560.0
76.00	1548.0
77.10	427.0
77.90	198.0
78.80	905.0
79.80	266.0
80.80	970.0
81.90	262.0
86.80	1787.0
87.70	1393.0
90.80	169.0
91.80	1023.0
92.90	1358.0
93.90	3137.0
94.90	32768.0
95.90	2196.0
103.90	163.0
105.90	110.0
115.50	111.0
116.70	180.0
118.60	218.0
127.80	120.0
130.60	105.0
140.60	242.0
142.80	283.0
144.80	126.0
145.00	126.0
147.70	103.0
171.90	581.0
173.80	25768.0
174.80	1822.0
175.80	24912.0
176.80	1853.0
192.70	103.0
206.90	706.0
207.70	187.0
208.80	126.0
268.80	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	392.0
36.90	1469.0
37.90	1342.0
39.00	840.0
39.80	647.0
40.80	164.0
42.80	152.0
43.90	1888.0
44.90	414.0
46.90	579.0
47.70	272.0
48.80	1101.0
49.90	5718.0
50.90	1991.0
51.90	203.0
54.90	137.0
55.80	366.0
57.00	853.0
59.80	281.0
60.80	1704.0
61.90	1710.0
62.90	1575.0
63.80	308.0
64.90	475.0
66.80	151.0
67.90	3436.0
68.90	3600.0
69.90	300.0
72.00	261.0
72.90	1564.0
73.90	5717.0
74.90	16592.0
76.00	1768.0
77.00	416.0
77.90	241.0
78.80	1095.0
79.80	326.0
80.80	1023.0
81.90	209.0
86.80	1883.0
87.70	1473.0
90.80	171.0
91.80	1159.0
92.90	1433.0
93.90	3341.0
94.90	34296.0
95.90	2351.0
103.90	198.0
105.60	100.0
105.90	111.0
115.50	147.0
116.70	212.0
118.60	275.0
127.80	166.0
129.60	122.0
140.60	272.0
140.90	270.0
142.80	353.0
144.80	180.0
147.00	105.0
171.90	605.0
172.90	312.0
173.80	28896.0
174.80	2090.0
175.80	28152.0
176.80	1966.0
187.60	114.0
206.90	799.0
208.80	135.0
268.90	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	361.0
36.90	1435.0
37.90	1288.0
39.00	768.0
39.80	646.0
40.80	120.0
42.00	141.0
42.80	142.0
43.90	1885.0
44.90	415.0
46.90	500.0
47.60	261.0
48.80	1150.0
49.90	5439.0
50.90	1791.0
52.00	162.0
52.90	101.0
54.90	130.0
55.80	380.0
56.90	772.0
59.90	338.0
60.80	1631.0
61.90	1675.0
62.90	1397.0
63.90	315.0
64.90	443.0
66.80	195.0
67.90	3322.0
68.90	3627.0
69.90	256.0
72.00	327.0
72.80	1513.0
73.90	5489.0
74.90	16150.0
76.00	1677.0
76.90	368.0
77.90	275.0
78.80	1134.0
79.90	350.0
80.80	946.0
81.80	187.0
86.90	1838.0
87.80	1490.0
90.80	132.0
91.80	1068.0
92.80	1384.0
93.90	3477.0
94.90	33184.0
95.90	2275.0
103.90	189.0
115.50	121.0
116.70	233.0
118.60	311.0
127.80	150.0
129.60	126.0
141.00	362.0
142.80	434.0
144.80	218.0
171.80	577.0
172.90	341.0
173.80	29080.0
174.80	1963.0
175.80	28256.0
176.80	1938.0
192.90	124.0
206.90	804.0
208.90	106.0
269.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76