


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV080320\
 Data File : VV017789.D
 Acq On : 03 Aug 2020 11:14
 Operator : SY/MD
 Sample : BFB401
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB401

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 04 02:09:42 2020

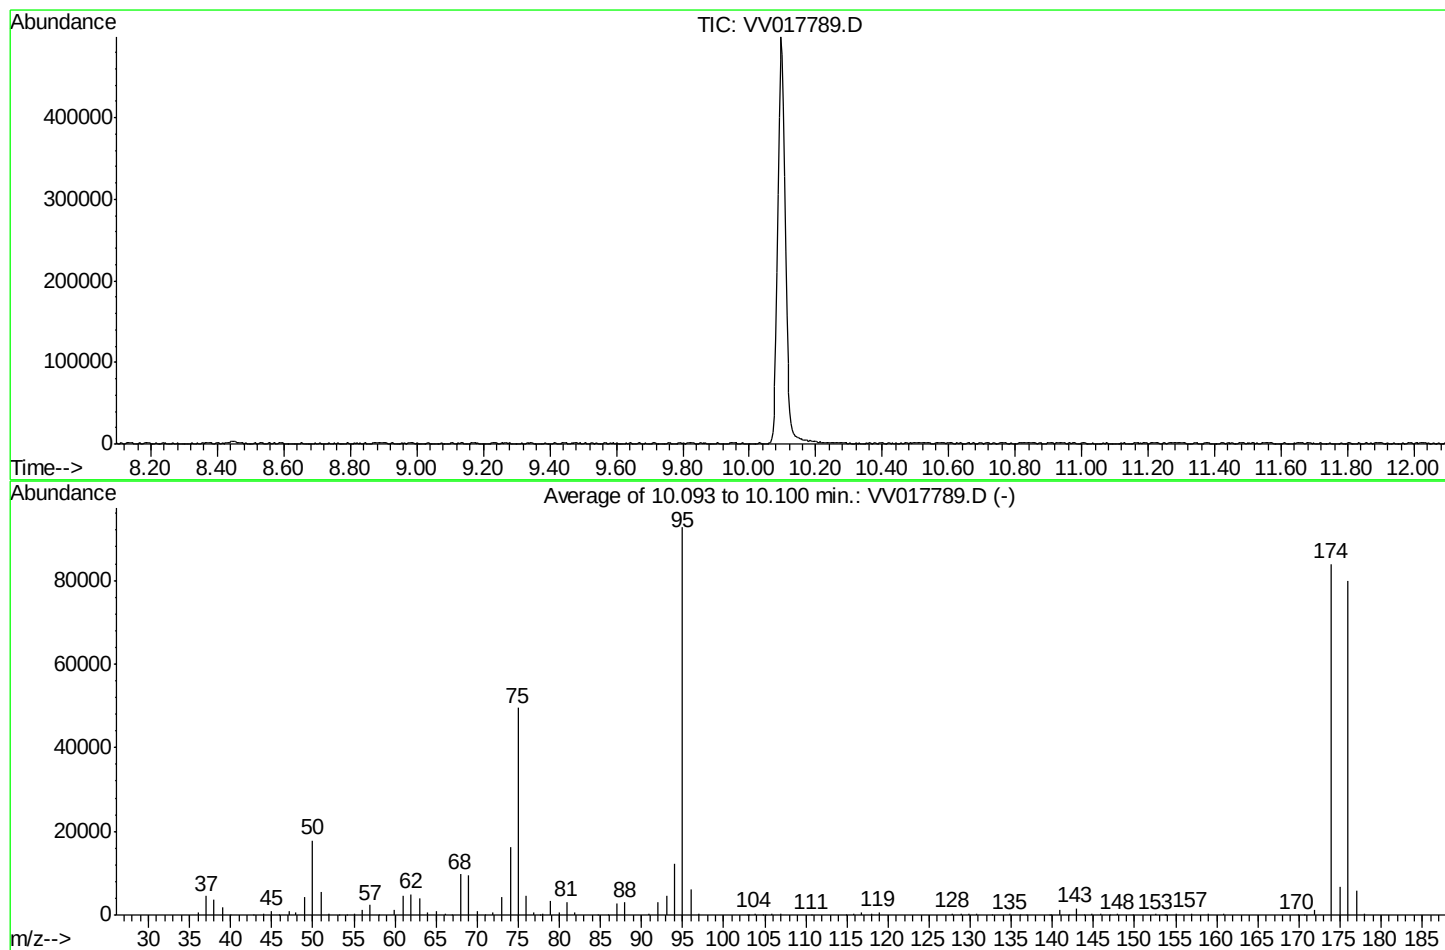

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	17869	PASS
75	95	30	80	53.5	49554	PASS
95	95	100	100	100.0	92682	PASS
96	95	5	9	6.7	6169	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.5	83861	PASS
175	174	5	9	8.1	6805	PASS
176	174	95	101	95.4	79965	PASS
177	176	5	9	7.1	5673	PASS

m/z	Abundance
36.10	647.0
37.10	4336.0
38.00	3926.0
39.00	1911.0
39.90	225.0
42.80	145.0
43.90	732.0
44.90	813.0
45.90	241.0
47.10	603.0
47.90	680.0
49.00	4237.0
50.00	17840.0
51.00	5382.0
51.90	316.0
53.10	224.0
54.20	113.0
55.00	342.0
56.00	1290.0
57.00	2340.0
58.10	159.0
59.90	1109.0
61.00	4699.0
62.00	4773.0
63.00	4018.0
64.00	591.0
65.10	937.0
66.10	238.0
68.00	9599.0
69.00	9701.0
70.10	925.0
71.00	124.0
71.90	678.0
73.00	3932.0
74.00	16070.0
75.00	48240.0
76.00	4579.0
76.90	492.0
78.00	436.0
78.90	3318.0
80.00	826.0
80.90	3127.0
81.90	705.0
84.70	106.0
85.90	147.0
87.00	2597.0
87.90	2926.0
90.90	378.0
92.00	3051.0
93.00	4545.0
94.00	12203.0
95.00	91216.0
96.00	6193.0
96.90	233.0
102.90	102.0
103.80	420.0
104.80	187.0
105.90	413.0
106.80	177.0
110.70	160.0
115.00	135.0
115.90	360.0
116.80	663.0
118.00	302.0
118.90	822.0
127.80	410.0
128.80	156.0
129.90	349.0
130.80	156.0
132.70	102.0
134.90	230.0
136.00	114.0
136.90	116.0
139.90	137.0
140.90	1146.0
141.90	162.0
142.80	1600.0
144.80	311.0
145.90	268.0
146.90	115.0
147.90	213.0
149.80	182.0
152.70	176.0
153.60	128.0
155.10	297.0
157.00	328.0
158.90	174.0
160.90	170.0
169.80	129.0
170.80	145.0
171.90	1135.0
173.90	81024.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

175.00	6650.0
175.90	76712.0
177.00	5243.0
177.90	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

m/z	Abundance
36.10	716.0
37.00	4678.0
38.00	3784.0
39.00	2023.0
39.90	208.0
42.80	124.0
43.90	679.0
45.00	962.0
46.00	243.0
47.10	899.0
47.90	702.0
49.00	4500.0
50.00	18512.0
51.00	5745.0
52.00	307.0
53.20	179.0
55.00	435.0
56.00	1300.0
57.00	2542.0
58.10	159.0
59.90	1160.0
61.00	4724.0
62.00	5226.0
63.00	4066.0
64.00	625.0
65.10	925.0
66.10	262.0
66.90	185.0
68.00	10051.0
69.00	9924.0
70.00	1041.0
71.90	690.0
73.00	4265.0
74.00	16920.0
75.00	51224.0
76.00	4850.0
77.00	505.0
78.00	334.0
78.90	3356.0
80.00	750.0
80.90	3202.0
81.90	600.0
85.90	117.0
87.00	2812.0
87.90	3006.0
90.80	437.0
92.00	3437.0
93.00	4918.0
94.00	12776.0
95.00	96104.0
96.00	6489.0
96.90	248.0
103.10	122.0
103.80	485.0
105.00	163.0
105.90	372.0
106.90	173.0
110.80	142.0
115.00	152.0
115.90	354.0
116.80	712.0
118.00	365.0
118.90	770.0
127.90	484.0
128.90	184.0
129.90	439.0
130.70	196.0
134.90	226.0
136.90	135.0
139.80	141.0
140.90	1252.0
142.00	169.0
142.80	1654.0
143.90	100.0
144.80	339.0
145.90	280.0
147.00	130.0
147.90	236.0
149.80	155.0
152.70	186.0
153.60	116.0
155.00	319.0
156.90	354.0
158.90	170.0
160.80	200.0
169.80	166.0
170.60	166.0
171.80	1267.0
173.90	86520.0
175.00	7070.0
175.90	82560.0
177.00	5857.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

177.90

224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

m/z	Abundance
36.10	792.0
37.00	4436.0
38.00	3400.0
39.00	1940.0
39.90	187.0
44.00	638.0
45.10	1003.0
46.00	181.0
47.10	1014.0
47.90	685.0
49.00	4188.0
50.00	17256.0
51.00	5663.0
52.00	344.0
55.10	413.0
55.90	1341.0
57.00	2471.0
57.90	114.0
59.90	1086.0
61.00	4332.0
62.00	5038.0
63.00	3979.0
64.00	689.0
65.10	851.0
66.10	189.0
68.00	9520.0
69.00	9181.0
70.00	1003.0
71.90	593.0
73.00	4342.0
74.00	16072.0
75.00	49200.0
76.00	4563.0
76.90	499.0
77.70	243.0
78.90	3009.0
80.00	687.0
80.90	2955.0
81.90	462.0
87.10	2588.0
88.00	2936.0
90.80	414.0
92.00	3172.0
93.10	4769.0
94.00	12025.0
95.00	90728.0
96.00	5826.0
96.90	250.0
103.10	142.0
103.80	449.0
105.00	171.0
105.80	346.0
107.00	173.0
110.80	108.0
114.90	146.0
115.80	356.0
116.80	741.0
118.00	367.0
118.90	694.0
127.90	465.0
128.80	211.0
129.90	448.0
130.60	181.0
134.80	215.0
136.90	159.0
139.60	163.0
140.90	1179.0
142.90	1611.0
143.80	128.0
144.90	364.0
145.90	310.0
146.80	115.0
148.00	273.0
149.90	112.0
152.60	164.0
153.90	113.0
155.00	324.0
156.90	331.0
158.90	152.0
160.80	216.0
169.80	164.0
170.60	166.0
171.80	1256.0
174.00	84040.0
175.00	6697.0
176.00	80624.0
177.00	5920.0
178.00	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

Scan 2788 (10.055 min): VV017789.D
BFB401

m/z	Abundance
39.60	146.0
40.00	133.0
44.00	217.0
45.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401