

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080321\
 Data File : VV021725.D
 Acq On : 03 Aug 2021 10:46
 Operator : SY/MD
 Sample : VV0803WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Quant Time: Aug 04 01:12:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 04 01:10:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	403185	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	374713	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	179162	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	103814	41.000	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.000%	
7) Chloroethane-d5	1.558	69	95010	45.496	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.000%	
11) 1,1-Dichloroethene-d2	2.102	63	154322	34.077	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.160%	
21) 2-Butanone-d5	3.870	46	218863	100.626	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.630%	
24) Chloroform-d	4.346	84	243898	45.446	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.900%	
26) 1,2-Dichloroethane-d4	5.031	65	153939	47.963	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.920%	
32) Benzene-d6	5.050	84	512632	48.268	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.540%	
36) 1,2-Dichloropropane-d6	6.069	67	165864	49.273	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.540%	
41) Toluene-d8	7.317	98	462999	47.118	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.240%	
43) trans-1,3-Dichloroprop...	7.622	79	75793	45.631	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.260%	
47) 2-Hexanone-d5	8.088	63	131824	89.810	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	89.810%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	200259	45.139	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.280%	
66) 1,2-Dichlorobenzene-d4	11.625	152	182798	49.278	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.560%	
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.140	43	14929	4.980	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080321\
Data File : VV021725.D
Acq On : 03 Aug 2021 10:46
Operator : SY/MD
Sample : VV0803WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Time: Aug 04 01:12:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 04 01:10:57 2021
Response via : Initial Calibration

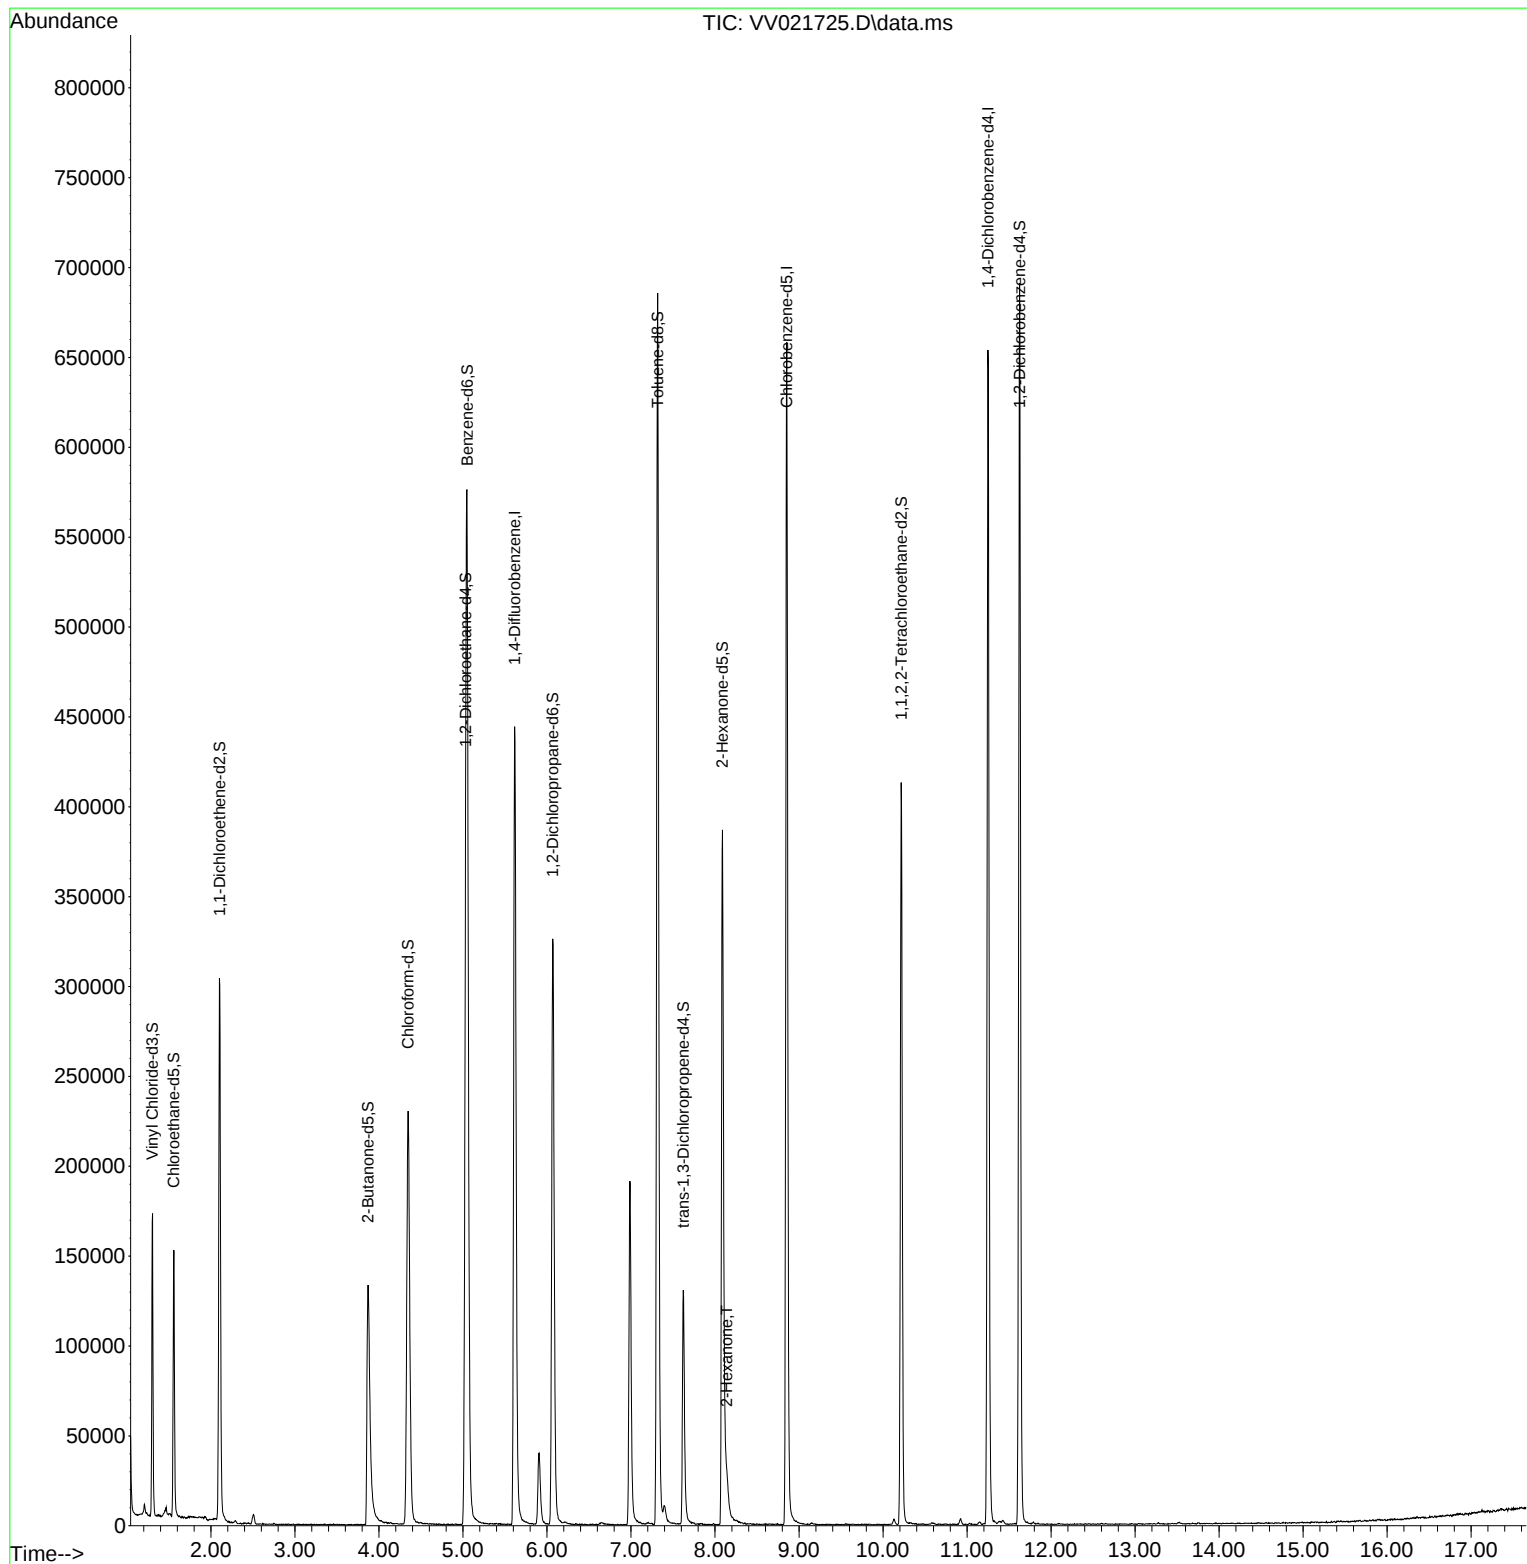

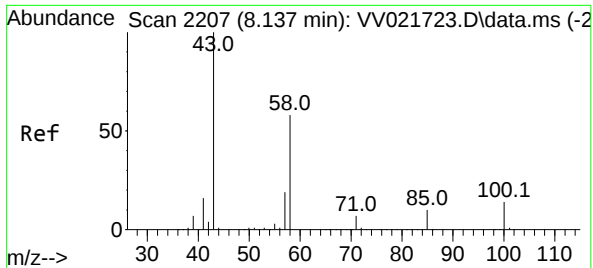

#48
 2-Hexanone
 Concen: 4.980 ug/L
 RT: 8.140 min Scan# 2208
 Delta R.T. 0.003 min
 Lab File: VV021725.D
 Acq: 03 Aug 2021 10:46

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Tgt Ion: 43	Resp: 14929
Ion Ratio	Lower Upper
43	100
58	39.4 46.0 69.0#
57	7.6 15.0 22.4#
100	8.9 11.1 16.7#

