
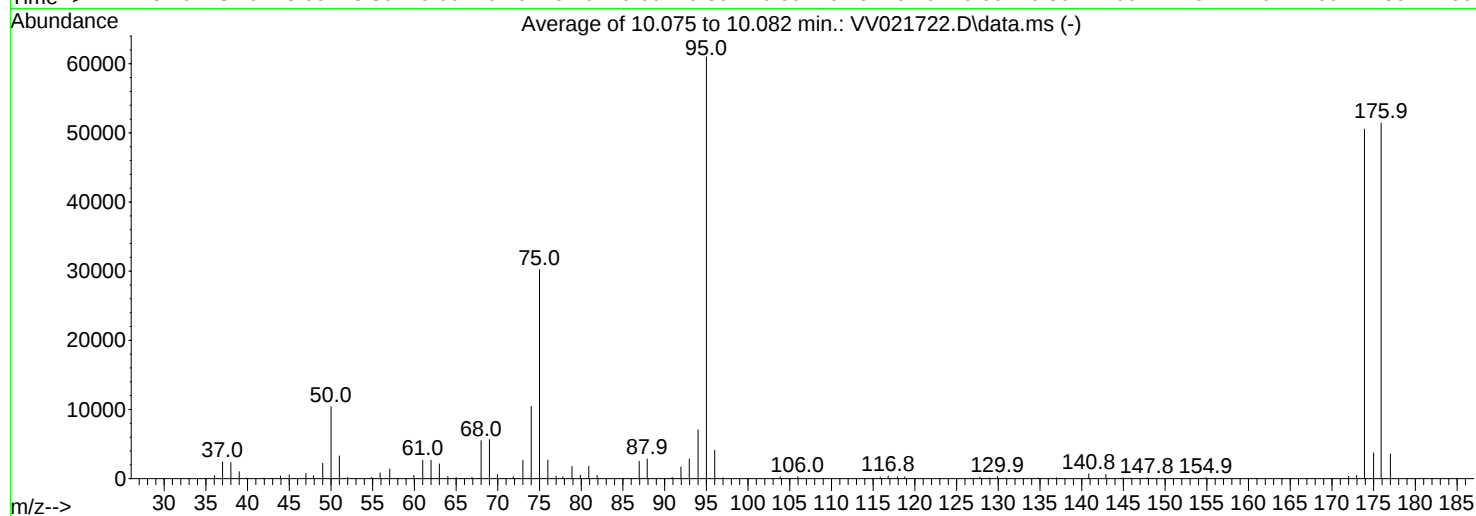


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080321\
 Data File : VV021722.D
 Acq On : 03 Aug 2021 09:01
 Operator : SY/MD
 Sample : BFB212
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB212

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 04 01:10:57 2021

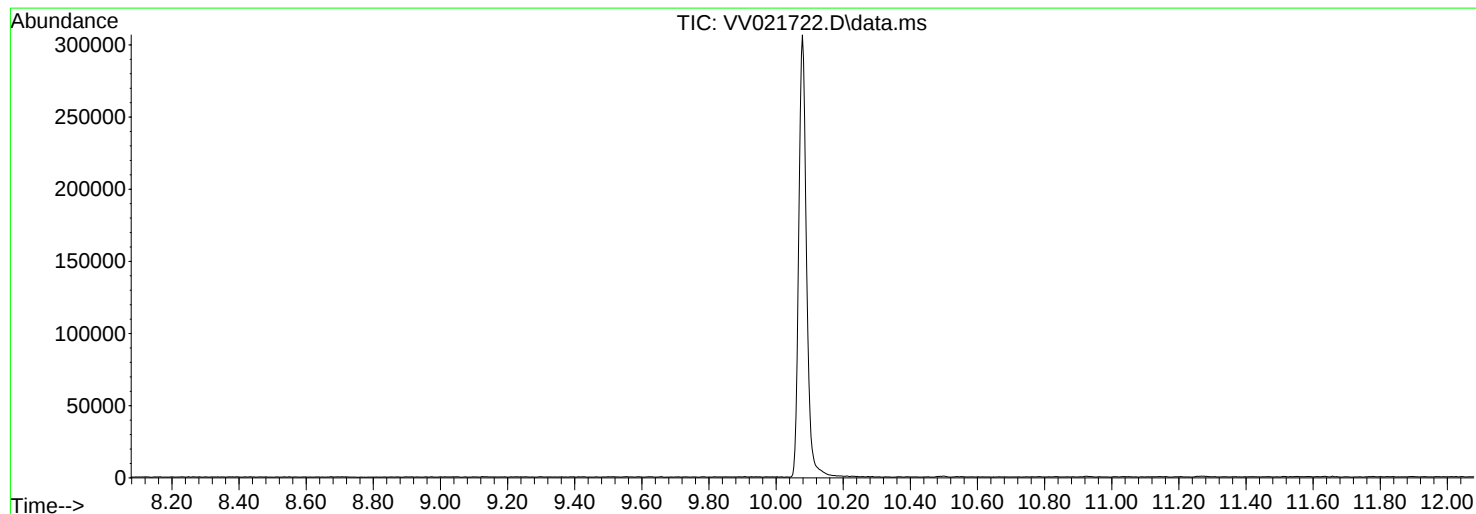

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	10406	PASS
75	95	30	80	49.5	30213	PASS
95	95	100	100	100.0	60992	PASS
96	95	5	9	6.7	4100	PASS
173	174	0.00	2	0.9	452	PASS
174	95	50	120	82.9	50565	PASS
175	174	5	9	7.4	3717	PASS
176	174	95	105	101.7	51424	PASS
177	176	5	10	6.9	3562	PASS

m/z	Abundance
39.90	172.0
43.90	390.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.00	452.0
37.00	2357.0
38.00	2399.0
39.00	948.0
39.80	252.0
42.90	103.0
44.00	735.0
45.00	594.0
47.00	750.0
47.90	379.0
49.00	2216.0
50.00	10476.0
51.00	3340.0
52.00	221.0
54.90	203.0
55.90	888.0
57.00	1357.0
58.00	129.0
59.90	495.0
61.00	2683.0
62.00	2737.0
63.00	2048.0
64.00	325.0
65.00	199.0
66.90	187.0
68.00	5472.0
69.00	5695.0
69.90	566.0
71.90	285.0
73.00	2562.0
74.00	10387.0
75.00	30488.0
76.00	2664.0
77.00	365.0
77.80	307.0
78.90	1729.0
79.90	484.0
80.90	1715.0
81.90	474.0
87.00	2553.0
87.90	2772.0
91.00	188.0
92.00	1562.0
93.00	2828.0
94.00	6969.0
95.00	60632.0
96.00	4125.0
97.00	160.0
103.90	259.0
104.90	106.0
106.00	243.0
115.80	210.0
116.80	363.0
117.90	302.0
118.80	289.0
127.80	200.0
128.90	146.0
129.90	299.0
134.80	108.0
137.00	137.0
140.80	723.0
142.90	626.0
144.90	108.0
145.80	115.0
148.00	110.0
154.90	151.0
172.00	329.0
173.00	413.0
173.90	49456.0
175.00	3698.0
175.90	49656.0
177.00	3531.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.10	465.0
37.00	2470.0
38.00	2447.0
39.00	1057.0
39.90	282.0
43.00	106.0
44.00	803.0
45.00	577.0
47.00	748.0
47.90	401.0
49.00	2278.0
50.00	10695.0
51.00	3429.0
52.00	189.0
54.90	183.0
55.90	872.0
57.10	1435.0
58.10	106.0
60.00	495.0
61.00	2730.0
62.00	2729.0
63.00	2202.0
64.00	347.0
65.00	205.0
66.90	221.0
68.00	5718.0
69.00	5838.0
70.00	611.0
71.80	266.0
73.00	2771.0
74.00	10854.0
75.00	31344.0
76.00	2748.0
77.00	401.0
77.80	263.0
78.90	1834.0
79.90	540.0
80.90	1855.0
81.90	496.0
87.00	2585.0
87.90	2993.0
90.90	207.0
91.90	1728.0
92.90	2981.0
94.00	7312.0
95.00	62888.0
96.00	4225.0
97.00	154.0
103.90	277.0
106.00	286.0
115.80	238.0
116.80	396.0
117.90	282.0
118.80	295.0
127.80	215.0
128.90	131.0
129.90	320.0
130.90	113.0
134.80	112.0
137.00	138.0
140.90	746.0
142.90	633.0
144.90	110.0
147.80	146.0
154.90	167.0
156.70	115.0
160.90	104.0
172.00	385.0
172.90	443.0
173.90	52192.0
175.00	3875.0
175.90	53368.0
177.00	3684.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.10	419.0
37.00	2420.0
38.00	2180.0
39.00	1021.0
39.90	264.0
41.90	110.0
42.90	104.0
44.00	808.0
45.00	492.0
47.00	704.0
47.90	440.0
49.00	2162.0
50.00	10047.0
51.00	3110.0
52.00	143.0
54.90	172.0
55.90	719.0
57.00	1378.0
60.00	470.0
61.00	2515.0
62.00	2537.0
63.00	2124.0
64.00	279.0
65.00	188.0
66.90	232.0
68.00	5367.0
69.00	5406.0
70.00	575.0
71.80	281.0
73.00	2559.0
74.00	10159.0
75.00	28808.0
76.00	2626.0
77.00	353.0
77.80	240.0
78.90	1749.0
79.90	522.0
80.90	1789.0
81.90	456.0
86.90	2369.0
87.90	2747.0
90.80	231.0
91.90	1761.0
92.90	2701.0
94.00	6908.0
95.00	59456.0
96.00	3951.0
97.00	158.0
103.80	261.0
104.60	101.0
104.90	101.0
105.90	277.0
115.90	216.0
116.80	405.0
117.90	231.0
118.80	284.0
127.80	213.0
128.90	109.0
129.90	290.0
130.90	130.0
134.80	109.0
137.00	123.0
140.90	652.0
142.90	559.0
145.00	101.0
147.80	160.0
154.90	154.0
156.80	124.0
172.00	351.0
172.90	500.0
173.90	50048.0
175.00	3577.0
175.90	51248.0
177.00	3472.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212