

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
 Data File : VV006877.D
 Acq On : 04 Aug 2018 12:58
 Operator : SY/MD
 Sample : J4314-08
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KW6

Quant Time: Aug 06 03:39:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 03:23:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	257569	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	244176	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	94756	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	97877	5.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.80%
7) Chloroethane-d5	1.58	69	89507	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.40%
11) 1,1-Dichloroethene-d2	2.13	63	142454	4.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.20%
20) 2-Butanone-d5	3.97	46	229719	53.09	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.18%
24) Chloroform-d	4.41	84	175972	5.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.80%
26) 1,2-Dichloroethane-d4	5.09	65	90304	5.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.80%
32) Benzene-d6	5.11	84	332309	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	114562	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.20%
41) Toluene-d8	7.37	98	253714	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	7.67	79	34554	4.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.80%
46) 2-Hexanone-d5	8.15	63	137263	40.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	87005	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	89814	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	7391	2.42 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080418\
Data File : VV006877.D
Acq On : 04 Aug 2018 12:58
Operator : SY/MD
Sample : J4314-08
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KW6

Quant Time: Aug 06 03:39:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 03:23:10 2018
Response via : Initial Calibration

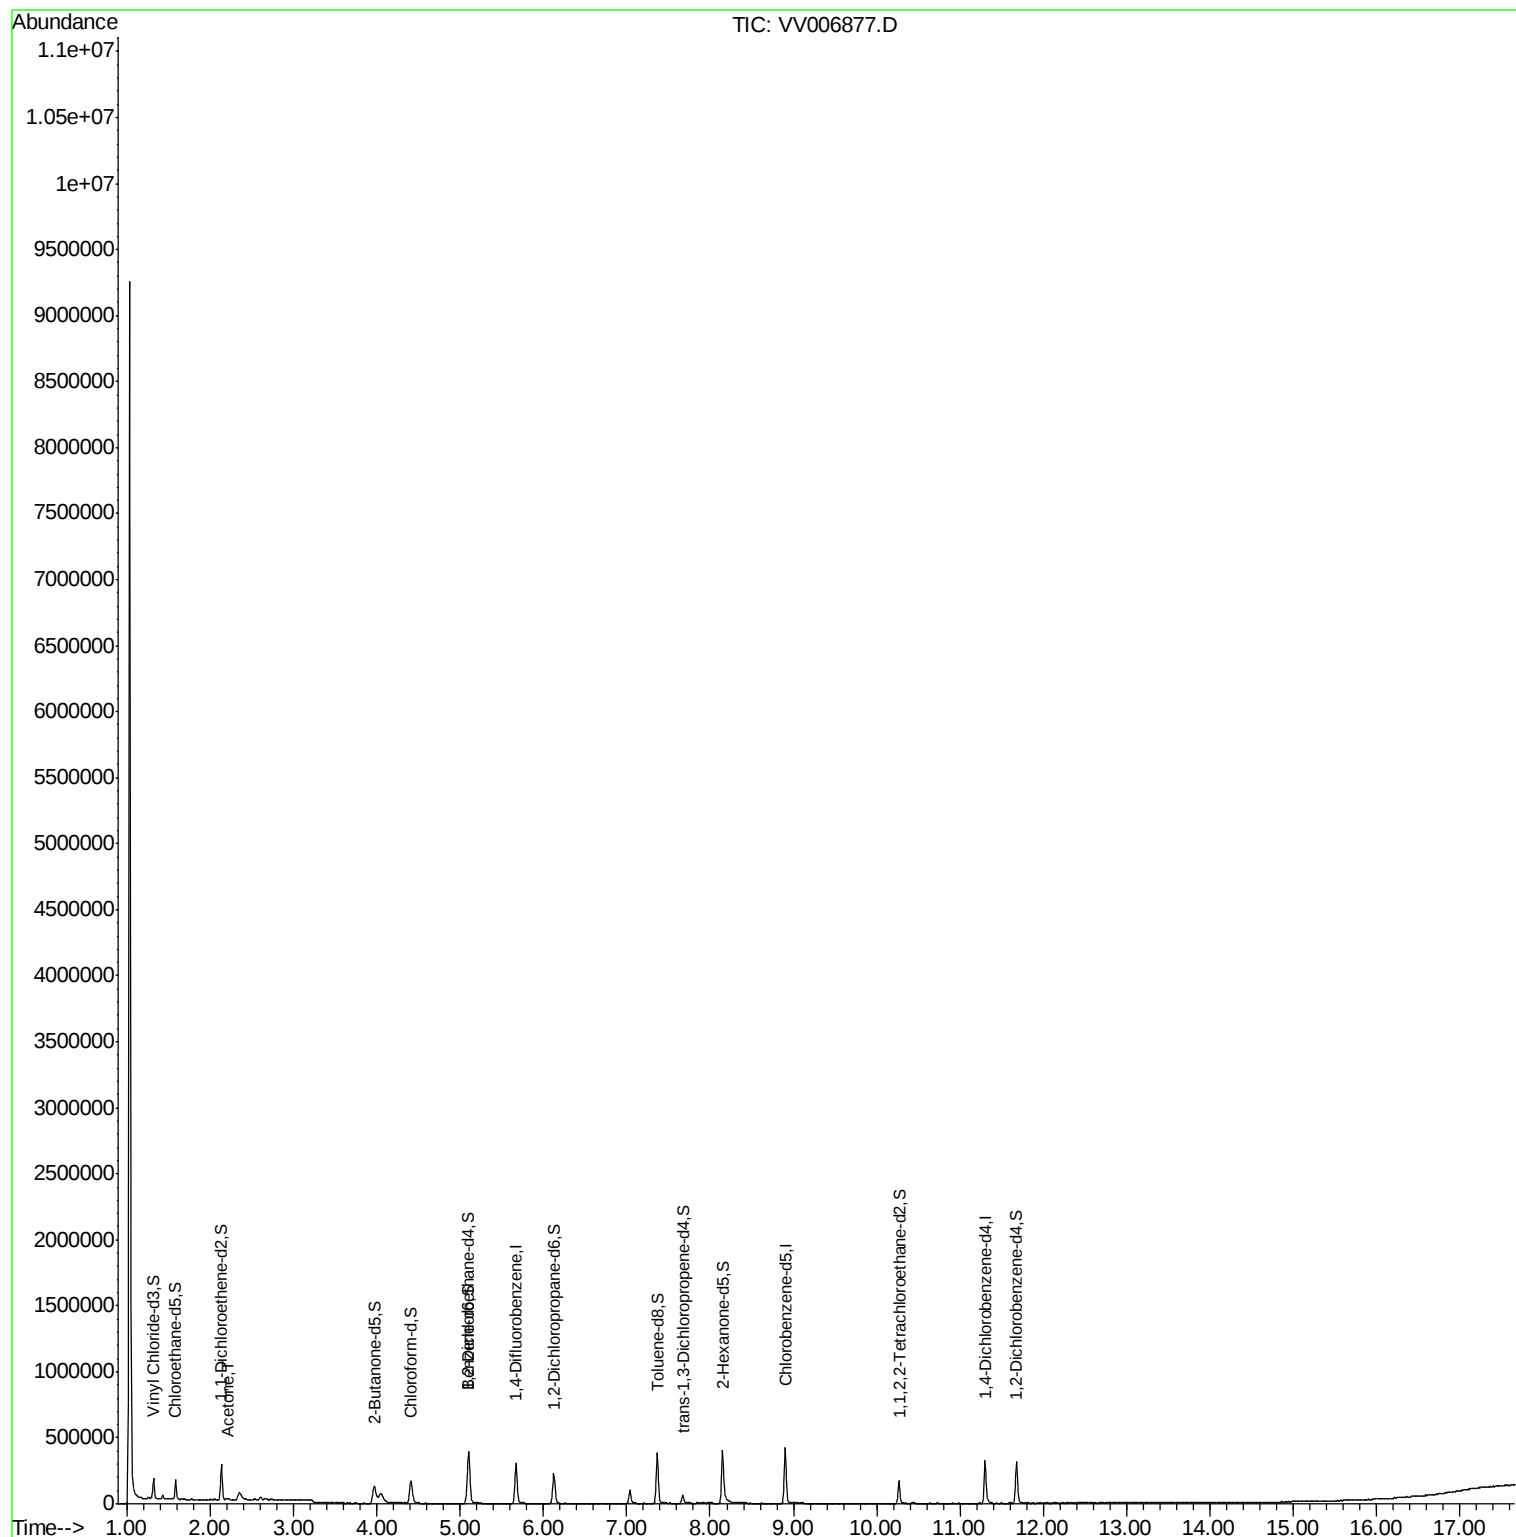

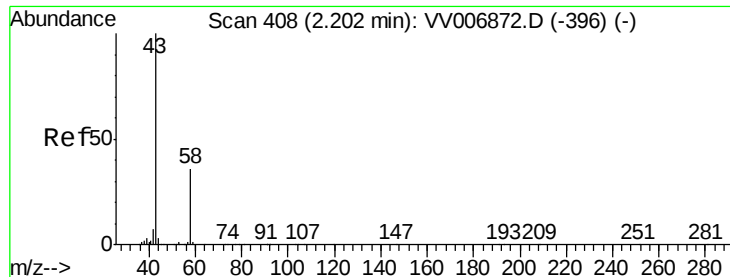

#13

Acetone

Concen: 2.42 ug/L

RT: 2.21 min Scan# 409

Delta R.T. 0.00 min

Lab File: VV006877.D

Acq: 04 Aug 2018 12:58

Instrument :
MSVOA_V
ClientSampleId :
C0KW6

Tot Ion: 43 Resp: 7391

Ion Ratio Lower Upper

43 100

58 35.7 0.0 69.0

