

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
 Data File : VV006886.D
 Acq On : 04 Aug 2018 16:58
 Operator : SY/MD
 Sample : J4314-17
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KX5

Quant Time: Aug 06 04:00:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 03:23:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	270942	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	258502	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	101322	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96789	5.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.20%
7) Chloroethane-d5	1.58	69	89869	5.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.20%
11) 1,1-Dichloroethene-d2	2.13	63	132232	3.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.00%
20) 2-Butanone-d5	3.97	46	237166	52.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.22%
24) Chloroform-d	4.40	84	177359	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
26) 1,2-Dichloroethane-d4	5.09	65	93599	5.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.00%
32) Benzene-d6	5.10	84	331663	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	115089	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.37	98	253432	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	7.67	79	34963	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.15	63	141054	38.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.74%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	88844	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	90280	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	7302	2.28 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080418\
Data File : VV006886.D
Acq On : 04 Aug 2018 16:58
Operator : SY/MD
Sample : J4314-17
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KX5

Quant Time: Aug 06 04:00:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 03:23:10 2018
Response via : Initial Calibration

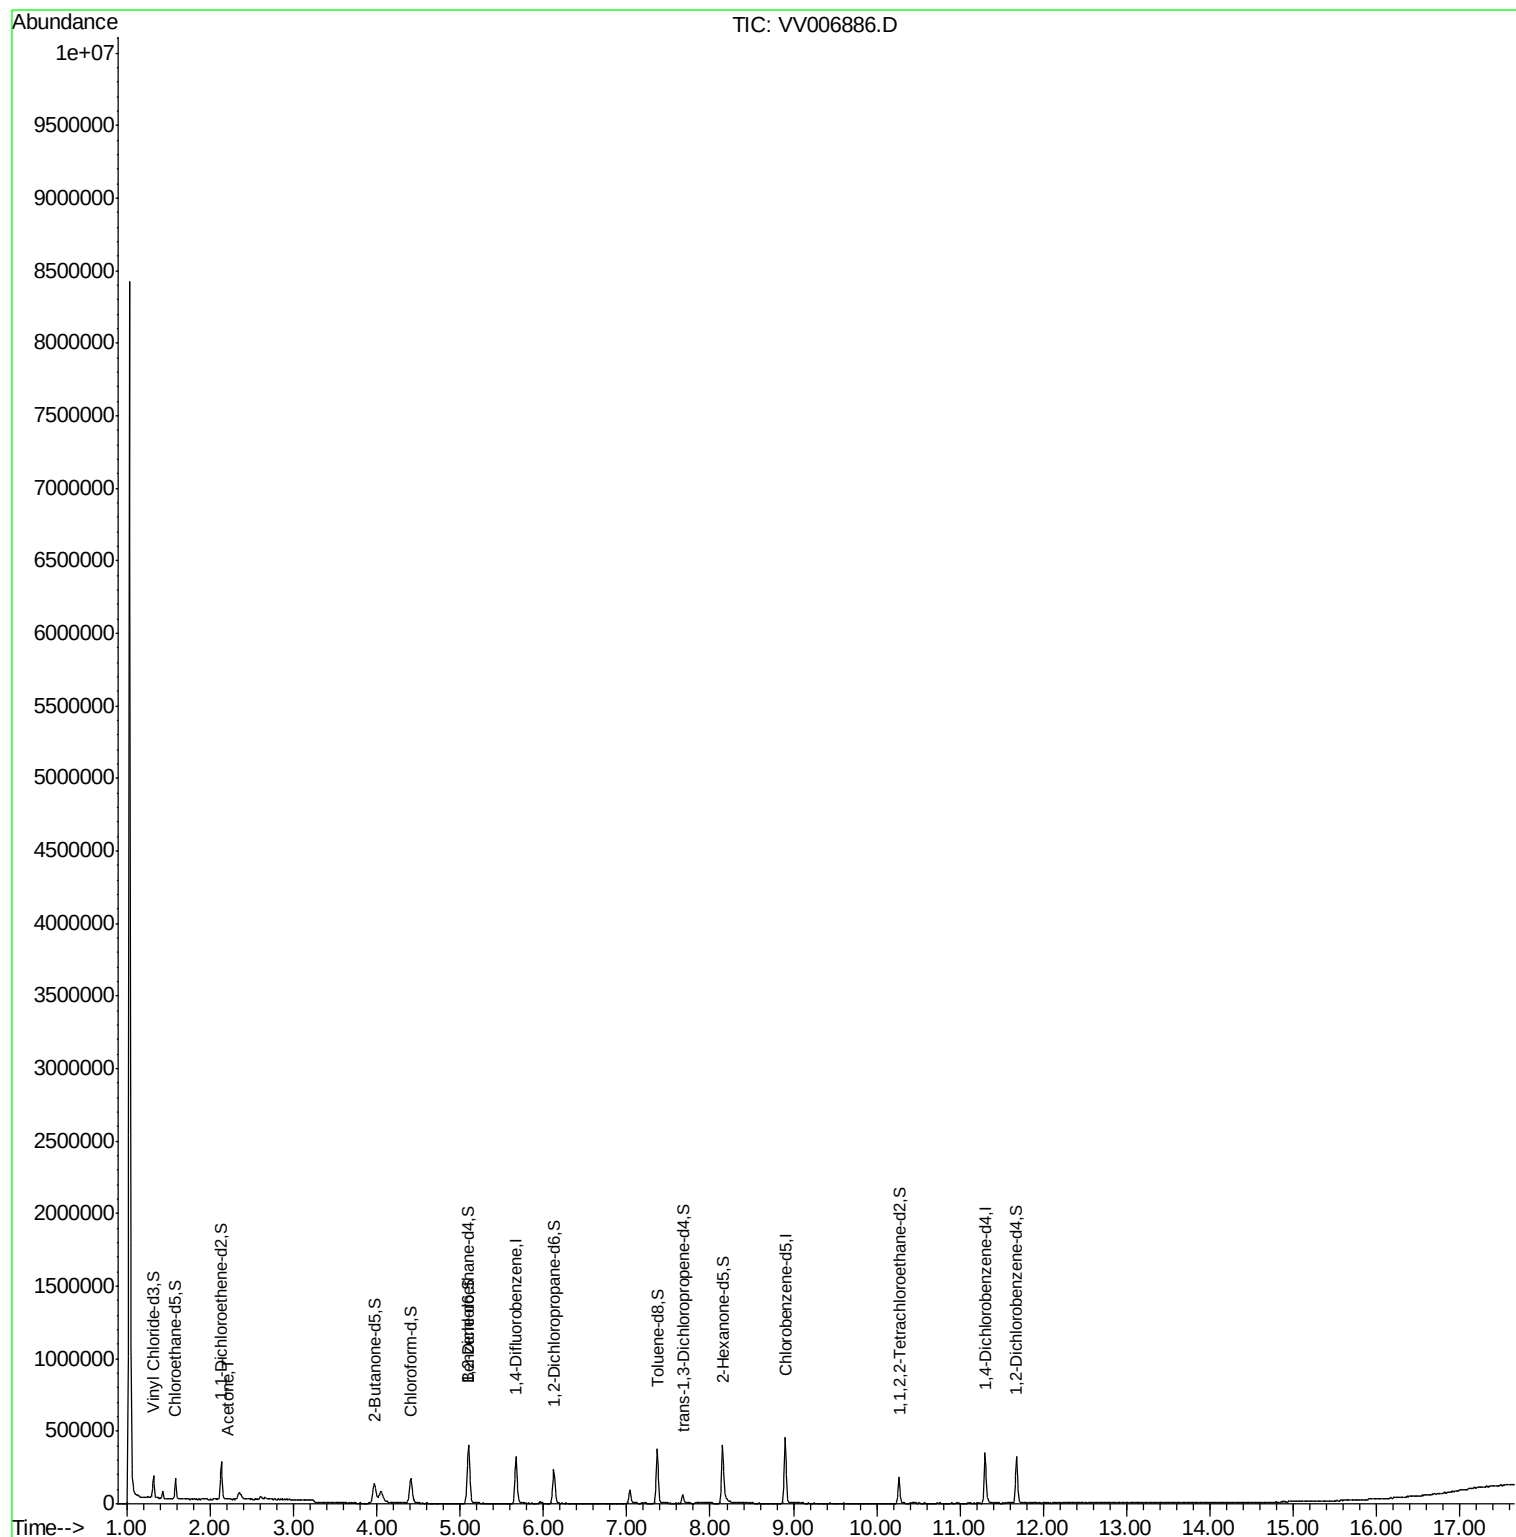

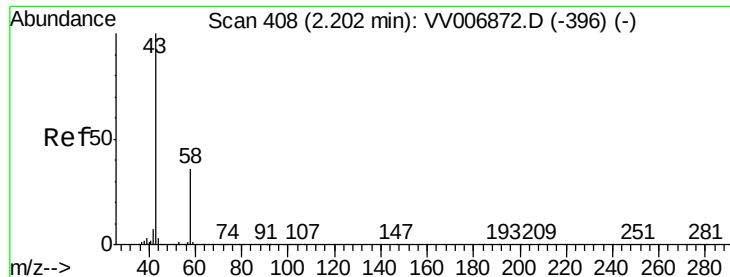

#13

Acetone

Concen: 2.28 ug/L

RT: 2.21 min Scan# 409

Delta R.T. 0.00 min

Lab File: VV006886.D

Acq: 04 Aug 2018 16:58

Instrument :
MSVOA_V
ClientSampleId :
C0KX5

Tot Ion: 43 Resp: 7302

Ion Ratio Lower Upper

43 100

58 35.2 0.0 69.0

