

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
 Data File : VV006889.D
 Acq On : 04 Aug 2018 18:19
 Operator : SY/MD
 Sample : J4314-20
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KX8

Quant Time: Aug 06 04:10:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 03:23:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	265637	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	257839	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	102530	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98223	5.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.80%
7) Chloroethane-d5	1.58	69	89171	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.40%
11) 1,1-Dichloroethene-d2	2.13	63	142652	4.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.60%
20) 2-Butanone-d5	3.97	46	270011	60.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.02%
24) Chloroform-d	4.41	84	182325	5.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.20%
26) 1,2-Dichloroethane-d4	5.09	65	96985	5.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.40%
32) Benzene-d6	5.10	84	338083	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.12	67	118686	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.36	98	258213	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	7.67	79	35759	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.15	63	164957	45.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.16%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	94619	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	92617	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	8622	2.74 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
Data File : VV006889.D
Acq On : 04 Aug 2018 18:19
Operator : SY/MD
Sample : J4314-20
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KX8

Quant Time: Aug 06 04:10:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 03:23:10 2018
Response via : Initial Calibration

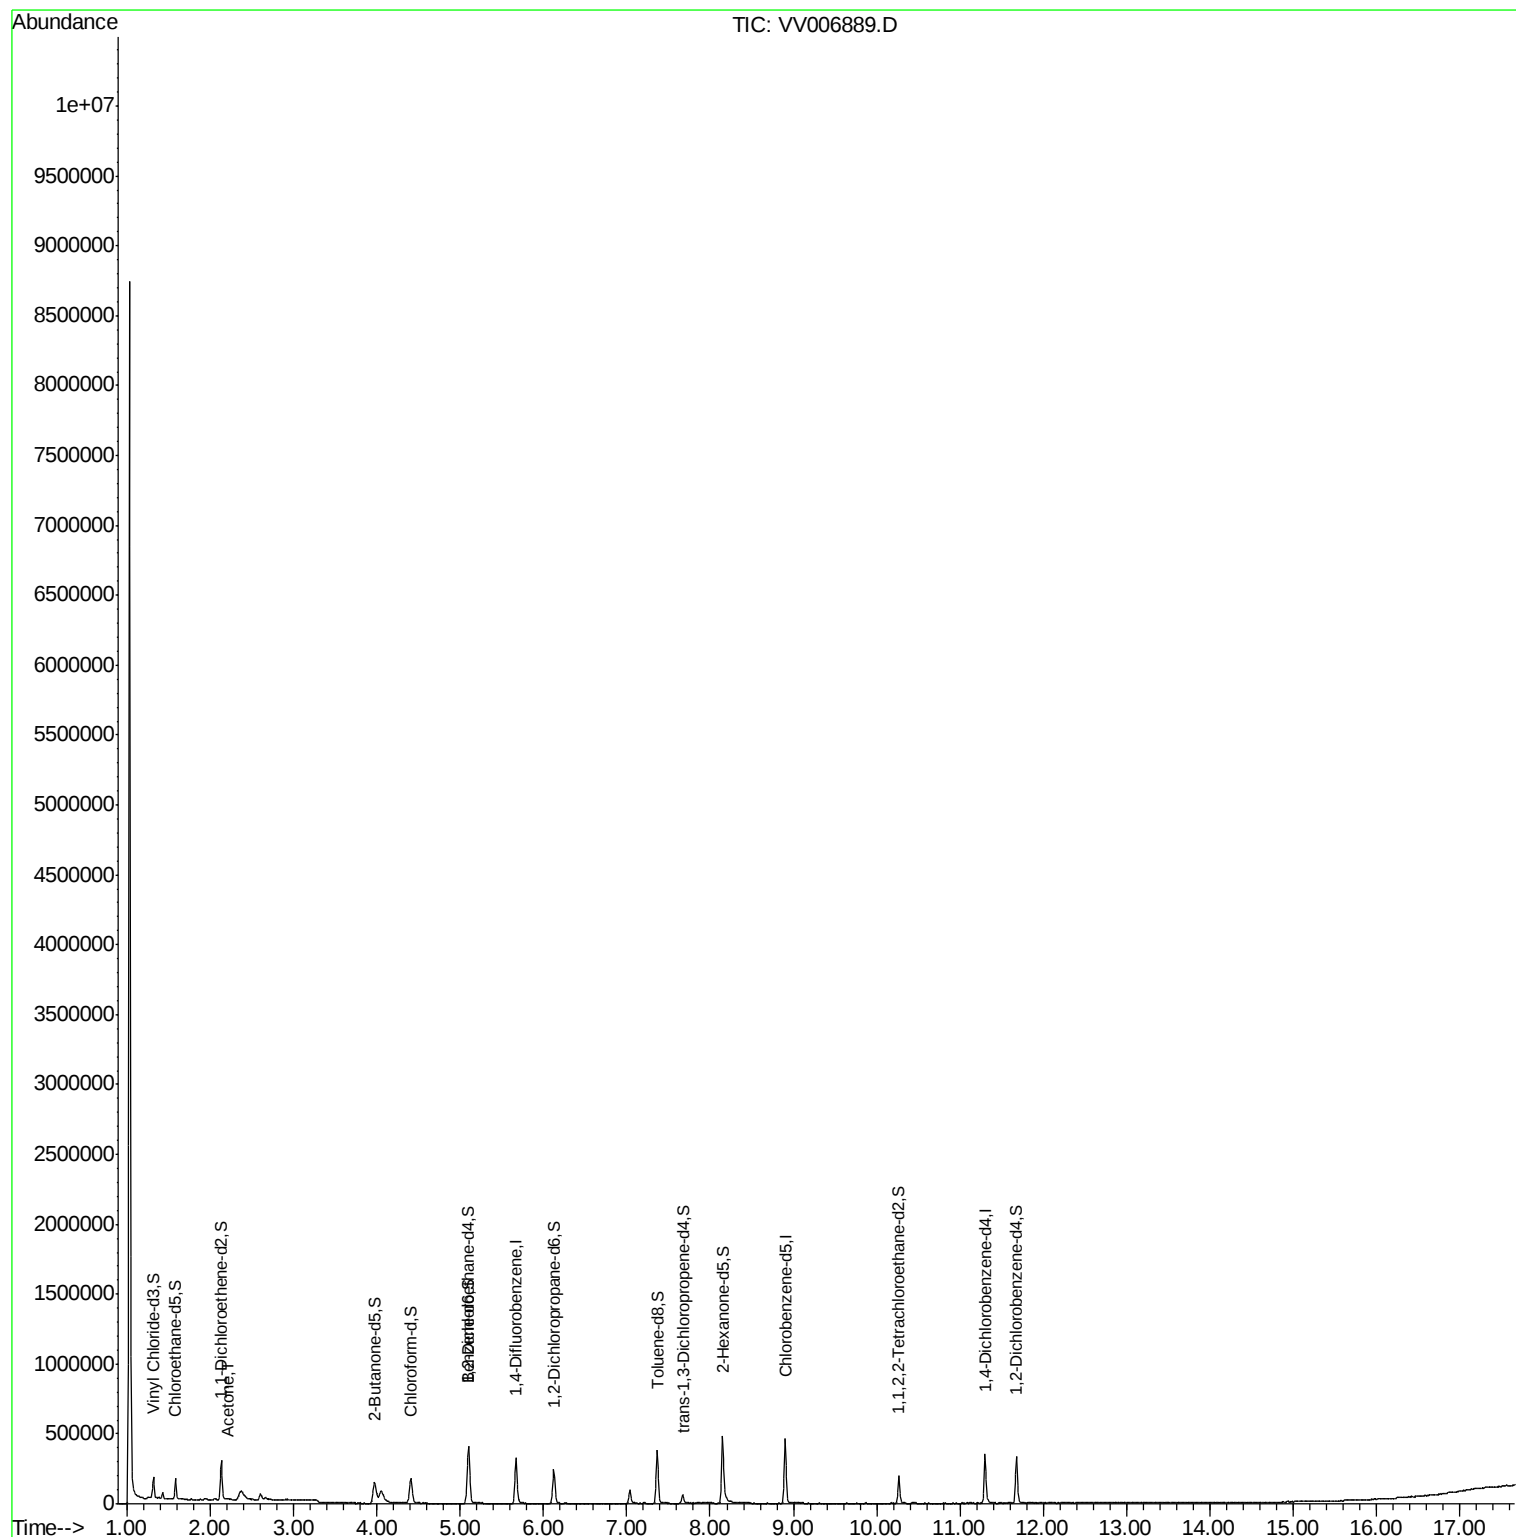

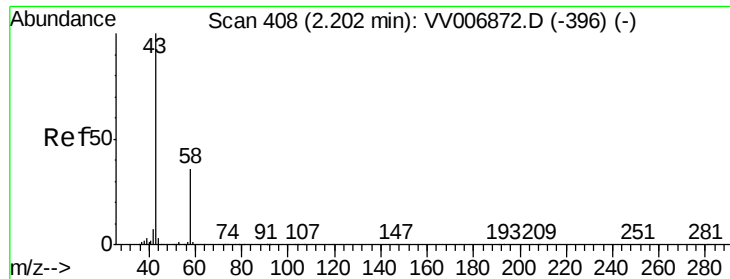

#13

Acetone

Concen: 2.74 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.01 min

Lab File: VV006889.D

Acq: 04 Aug 2018 18:19

Instrument :
MSVOA_V
ClientSampleId :
C0KX8

Tot Ion: 43 Resp: 8622

Ion Ratio Lower Upper

43 100

58 32.6 0.0 69.0

