

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
 Data File : VV006890.D
 Acq On : 04 Aug 2018 18:45
 Operator : SY/MD
 Sample : J4342-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E5F95

Quant Time: Aug 06 04:12:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 03:23:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	281479	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	271886	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	104562	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	99387	5.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.00%
7) Chloroethane-d5	1.58	69	92187	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.80%
11) 1,1-Dichloroethene-d2	2.13	63	145860	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.80%
20) 2-Butanone-d5	3.97	46	268096	56.70	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.40%
24) Chloroform-d	4.41	84	182833	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
26) 1,2-Dichloroethane-d4	5.09	65	97654	5.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.60%
32) Benzene-d6	5.10	84	347919	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.12	67	118766	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.37	98	254925	3.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.80%
43) trans-1,3-Dichloropropene-	7.67	79	35844	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.15	63	161229	42.25	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.50%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	95654	5.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	93234	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	42885	12.86 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
Data File : VV006890.D
Acq On : 04 Aug 2018 18:45
Operator : SY/MD
Sample : J4342-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E5F95

Quant Time: Aug 06 04:12:37 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 03:23:10 2018
Response via : Initial Calibration

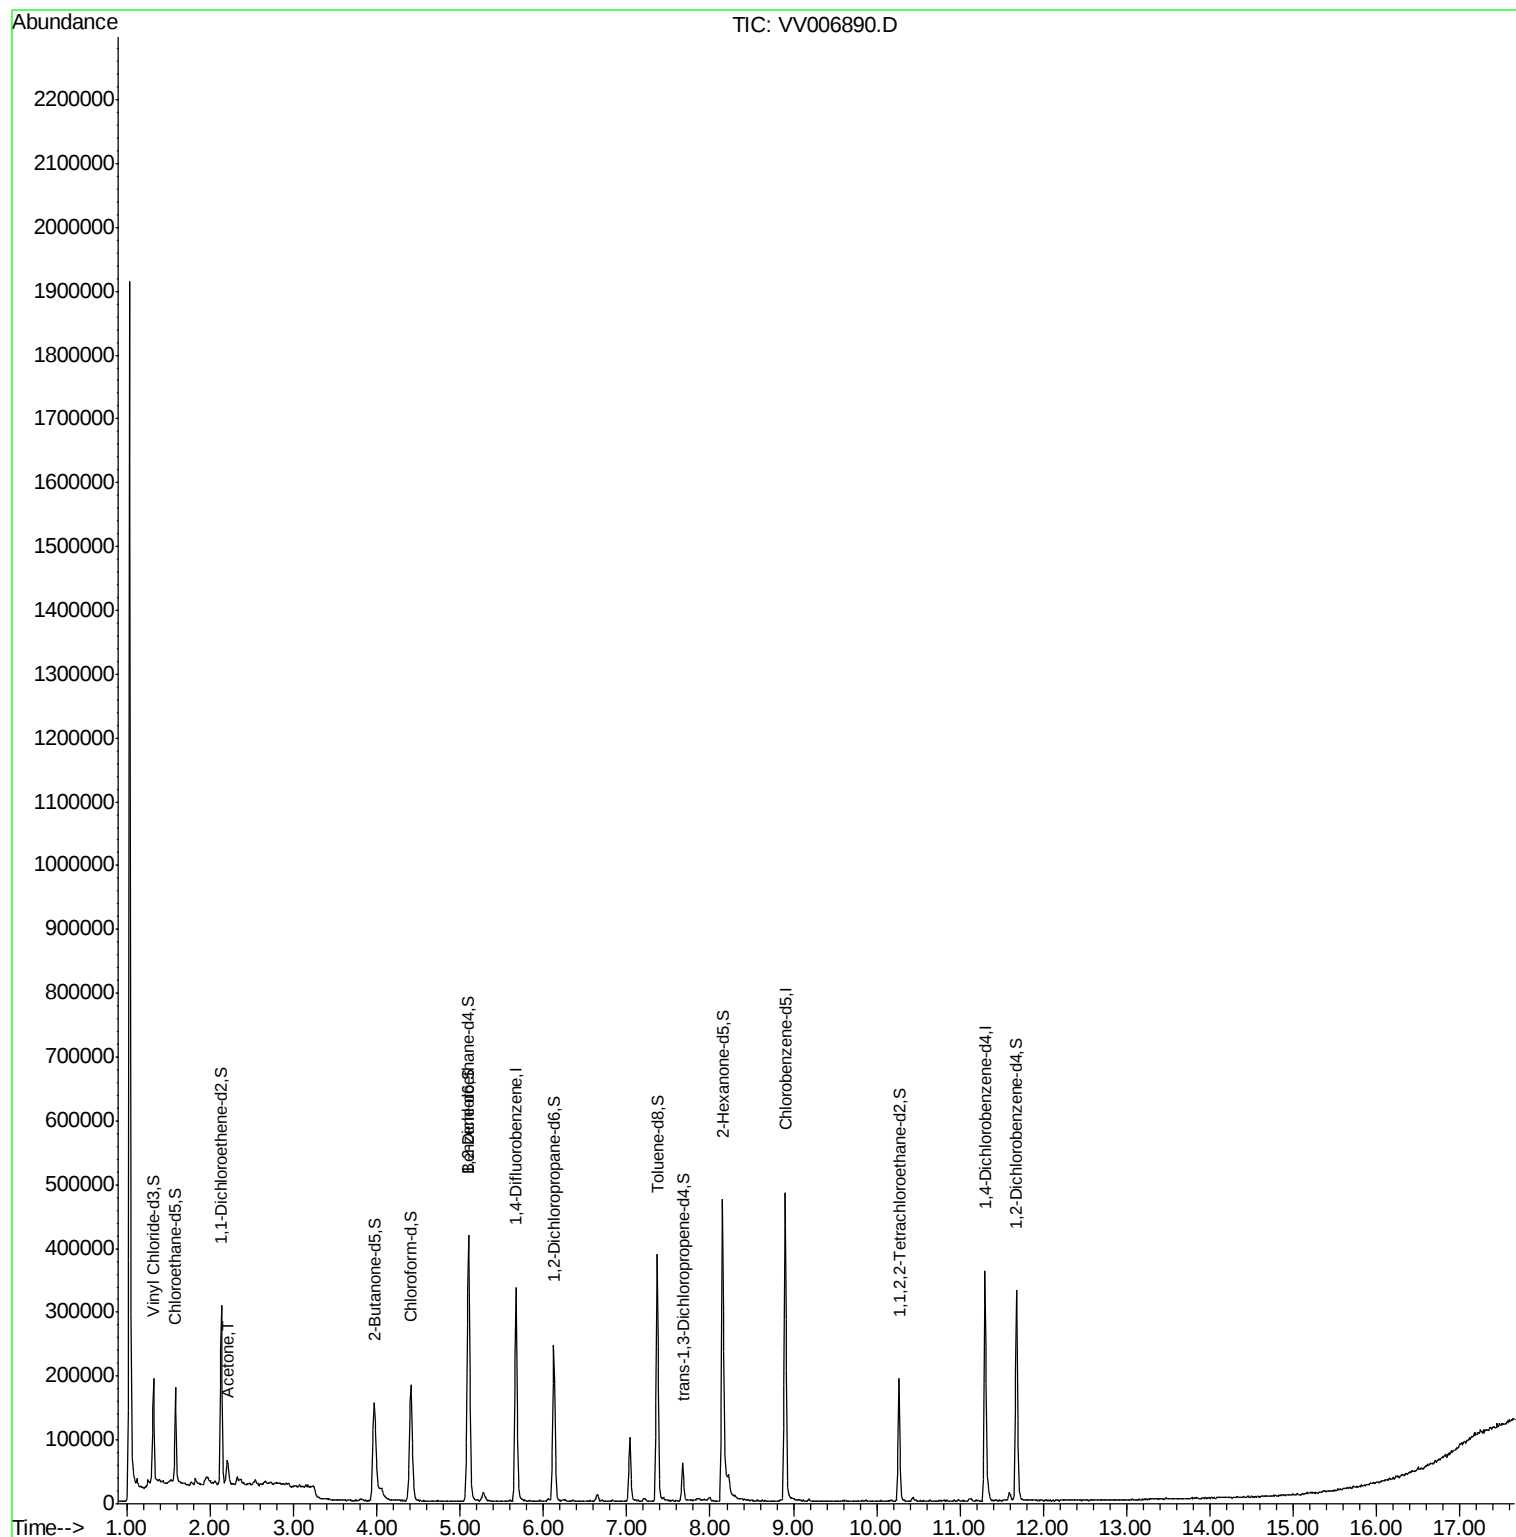

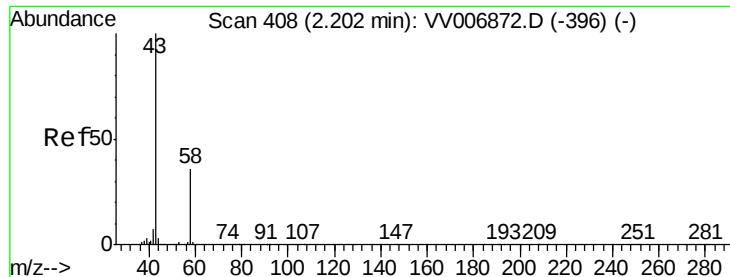

#13

Acetone

Concen: 12.86 ug/L

RT: 2.21 min Scan# 409

Delta R.T. 0.00 min

Lab File: VV006890.D

Acq: 04 Aug 2018 18:45

Instrument :
MSVOA_V
ClientSampleId :
E5F95

Tot Ion: 43 Resp: 42885

Ion Ratio Lower Upper

43 100

58 33.5 0.0 69.0

