


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080418\
 Data File : VV006871.D
 Acq On : 04 Aug 2018 09:05
 Operator : SY/MD
 Sample : BFB77
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 06 03:23:10 2018

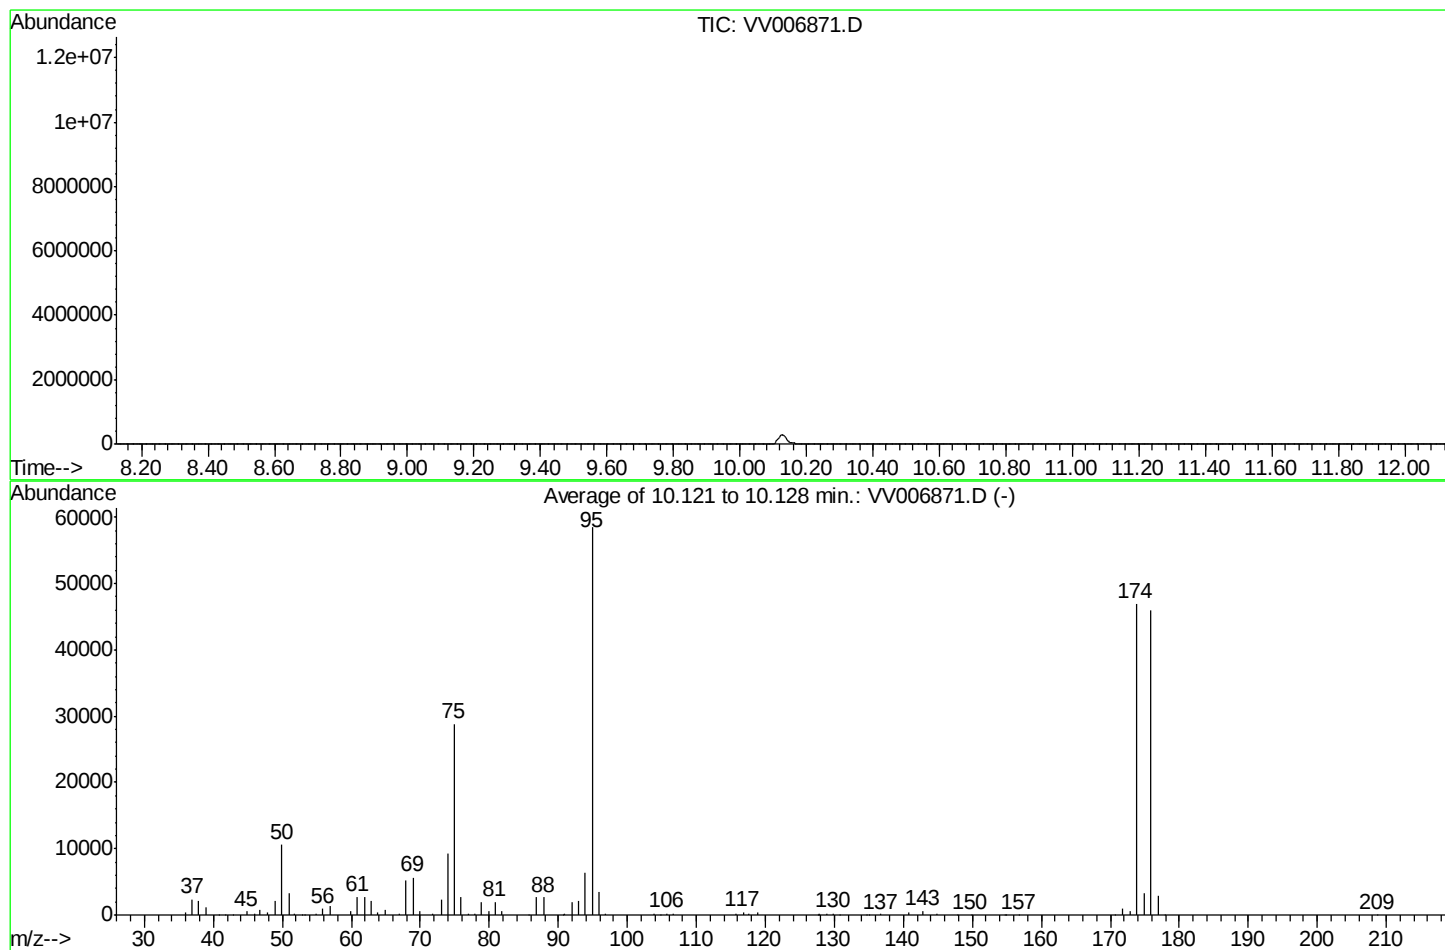

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10549	PASS
75	95	30	80	49.2	28781	PASS
95	95	100	100	100.0	58488	PASS
96	95	5	9	6.1	3542	PASS
173	174	0.00	2	1.1	496	PASS
174	95	50	120	80.2	46933	PASS
175	174	5	9	7.1	3325	PASS
176	174	95	101	97.9	45970	PASS
177	176	5	9	6.5	2985	PASS

Scan 2859 (10.083 min): VV006871.D
BFB77

m/z	Abundance
36.10	153.0
38.80	104.0
39.80	683.0
43.00	131.0
43.80	1853.0
44.90	134.0
76.90	240.0
78.00	140.0
132.90	138.0
206.90	568.0
269.00	138.0
280.80	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	553.0
36.90	2240.0
37.90	1911.0
38.90	1182.0
39.90	752.0
42.90	164.0
43.90	1732.0
44.80	691.0
46.00	113.0
46.80	700.0
47.90	363.0
48.90	2094.0
49.90	9657.0
50.90	3216.0
51.80	244.0
52.80	117.0
55.00	189.0
55.90	861.0
56.90	1321.0
60.00	569.0
60.90	2466.0
61.80	2512.0
62.90	1955.0
63.80	344.0
64.90	738.0
67.00	136.0
67.90	4721.0
68.90	5285.0
69.90	557.0
71.90	217.0
73.00	2088.0
73.90	8569.0
74.90	26640.0
75.90	2700.0
77.00	473.0
77.80	401.0
78.80	1725.0
79.90	539.0
80.80	1939.0
81.80	522.0
86.80	2352.0
87.90	2538.0
91.00	190.0
91.90	1878.0
92.90	2056.0
93.90	5717.0
94.90	54704.0
95.90	3231.0
96.80	179.0
103.80	200.0
104.80	141.0
105.80	266.0
106.60	122.0
115.60	187.0
116.90	358.0
117.60	194.0
118.80	404.0
127.60	159.0
127.90	159.0
128.90	139.0
129.90	237.0
130.80	118.0
136.70	119.0
140.70	408.0
142.90	570.0
144.80	206.0
155.00	138.0
171.80	762.0
172.80	449.0
173.80	41704.0
174.90	3148.0
175.80	41352.0
176.90	2578.0
206.90	482.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	630.0
36.90	2480.0
37.90	2239.0
38.90	1292.0
40.00	704.0
40.80	128.0
41.80	112.0
42.80	170.0
43.90	1756.0
44.90	673.0
46.00	170.0
46.80	746.0
47.90	432.0
48.90	2155.0
49.90	10779.0
51.00	3458.0
51.80	245.0
53.20	101.0
55.00	199.0
55.90	962.0
56.90	1291.0
59.90	686.0
60.90	2806.0
61.90	2662.0
62.90	2224.0
63.80	383.0
64.90	812.0
67.00	131.0
67.90	5355.0
68.90	5763.0
69.90	586.0
71.90	251.0
73.00	2497.0
73.90	9641.0
74.90	29880.0
75.90	2724.0
77.00	525.0
77.80	408.0
78.80	1931.0
79.90	618.0
80.80	2097.0
81.80	642.0
85.70	101.0
86.80	2737.0
87.90	2753.0
90.90	172.0
91.90	1952.0
92.90	2261.0
93.90	6497.0
94.90	60560.0
95.90	3651.0
96.80	252.0
103.90	228.0
104.80	131.0
105.80	255.0
106.60	177.0
115.60	217.0
116.90	436.0
117.60	205.0
118.80	381.0
127.80	159.0
128.90	143.0
129.90	264.0
134.60	134.0
135.10	105.0
136.80	148.0
140.70	479.0
142.90	654.0
144.80	231.0
147.80	129.0
149.80	108.0
154.90	111.0
156.70	133.0
171.80	951.0
172.90	525.0
173.80	48392.0
174.90	3419.0
175.80	47432.0
176.90	3064.0
206.90	505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	595.0
36.90	2496.0
37.90	2431.0
38.90	1277.0
39.80	575.0
40.80	128.0
41.80	137.0
42.80	163.0
43.90	1776.0
44.90	607.0
46.10	204.0
46.80	699.0
47.80	438.0
48.90	1986.0
49.90	11211.0
50.90	3221.0
51.80	223.0
53.20	101.0
54.90	151.0
55.90	940.0
56.90	1293.0
59.90	686.0
60.90	2894.0
61.90	2722.0
62.90	2258.0
63.90	337.0
64.90	818.0
67.00	117.0
67.90	5385.0
68.90	5803.0
69.90	605.0
71.80	250.0
73.00	2576.0
73.90	9678.0
74.90	29824.0
75.90	2559.0
77.00	557.0
77.80	381.0
78.80	2043.0
79.90	677.0
80.80	2036.0
81.80	654.0
85.70	167.0
86.80	2773.0
87.90	2667.0
90.70	194.0
91.90	1786.0
92.90	2257.0
93.90	6735.0
94.90	60200.0
95.90	3745.0
96.80	253.0
103.90	236.0
105.80	244.0
106.60	141.0
115.70	165.0
116.80	408.0
117.70	185.0
118.80	398.0
127.70	187.0
128.90	113.0
129.80	263.0
134.60	154.0
135.10	136.0
136.80	133.0
140.80	437.0
142.80	704.0
144.90	252.0
147.70	137.0
154.70	138.0
156.80	151.0
170.70	128.0
171.80	990.0
172.90	515.0
173.80	50704.0
174.90	3408.0
175.80	49128.0
176.90	3313.0
177.80	101.0
206.80	495.0
208.70	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77