

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080421\
 Data File : VV021733.D
 Acq On : 04 Aug 2021 11:24
 Operator : SY/MD
 Sample : VSTD1.015
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 05 02:31:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Aug 05 02:29:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	14115	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12988	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6422	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	7639	0.897	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	7709	1.066	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	10345	1.044	ug/L	0.00
8) Toluene-d8	7.317	98	29296	1.040	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	6214	1.127	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.303	62	13586	1.134	ug/L	99
6) Trichloroethene	5.925	95	11059	1.075	ug/L	99
9) 1,2-Dibromoethane	8.368	107	7009	1.072	ug/L	99
12) 1,2,3-Trichloropropane	10.267	75	5819	1.155	ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.426	75	787	0.978	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080421\
Data File : VV021733.D
Acq On : 04 Aug 2021 11:24
Operator : SY/MD
Sample : VSTD1.015
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 05 02:31:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 05 02:29:54 2021
Response via : Initial Calibration

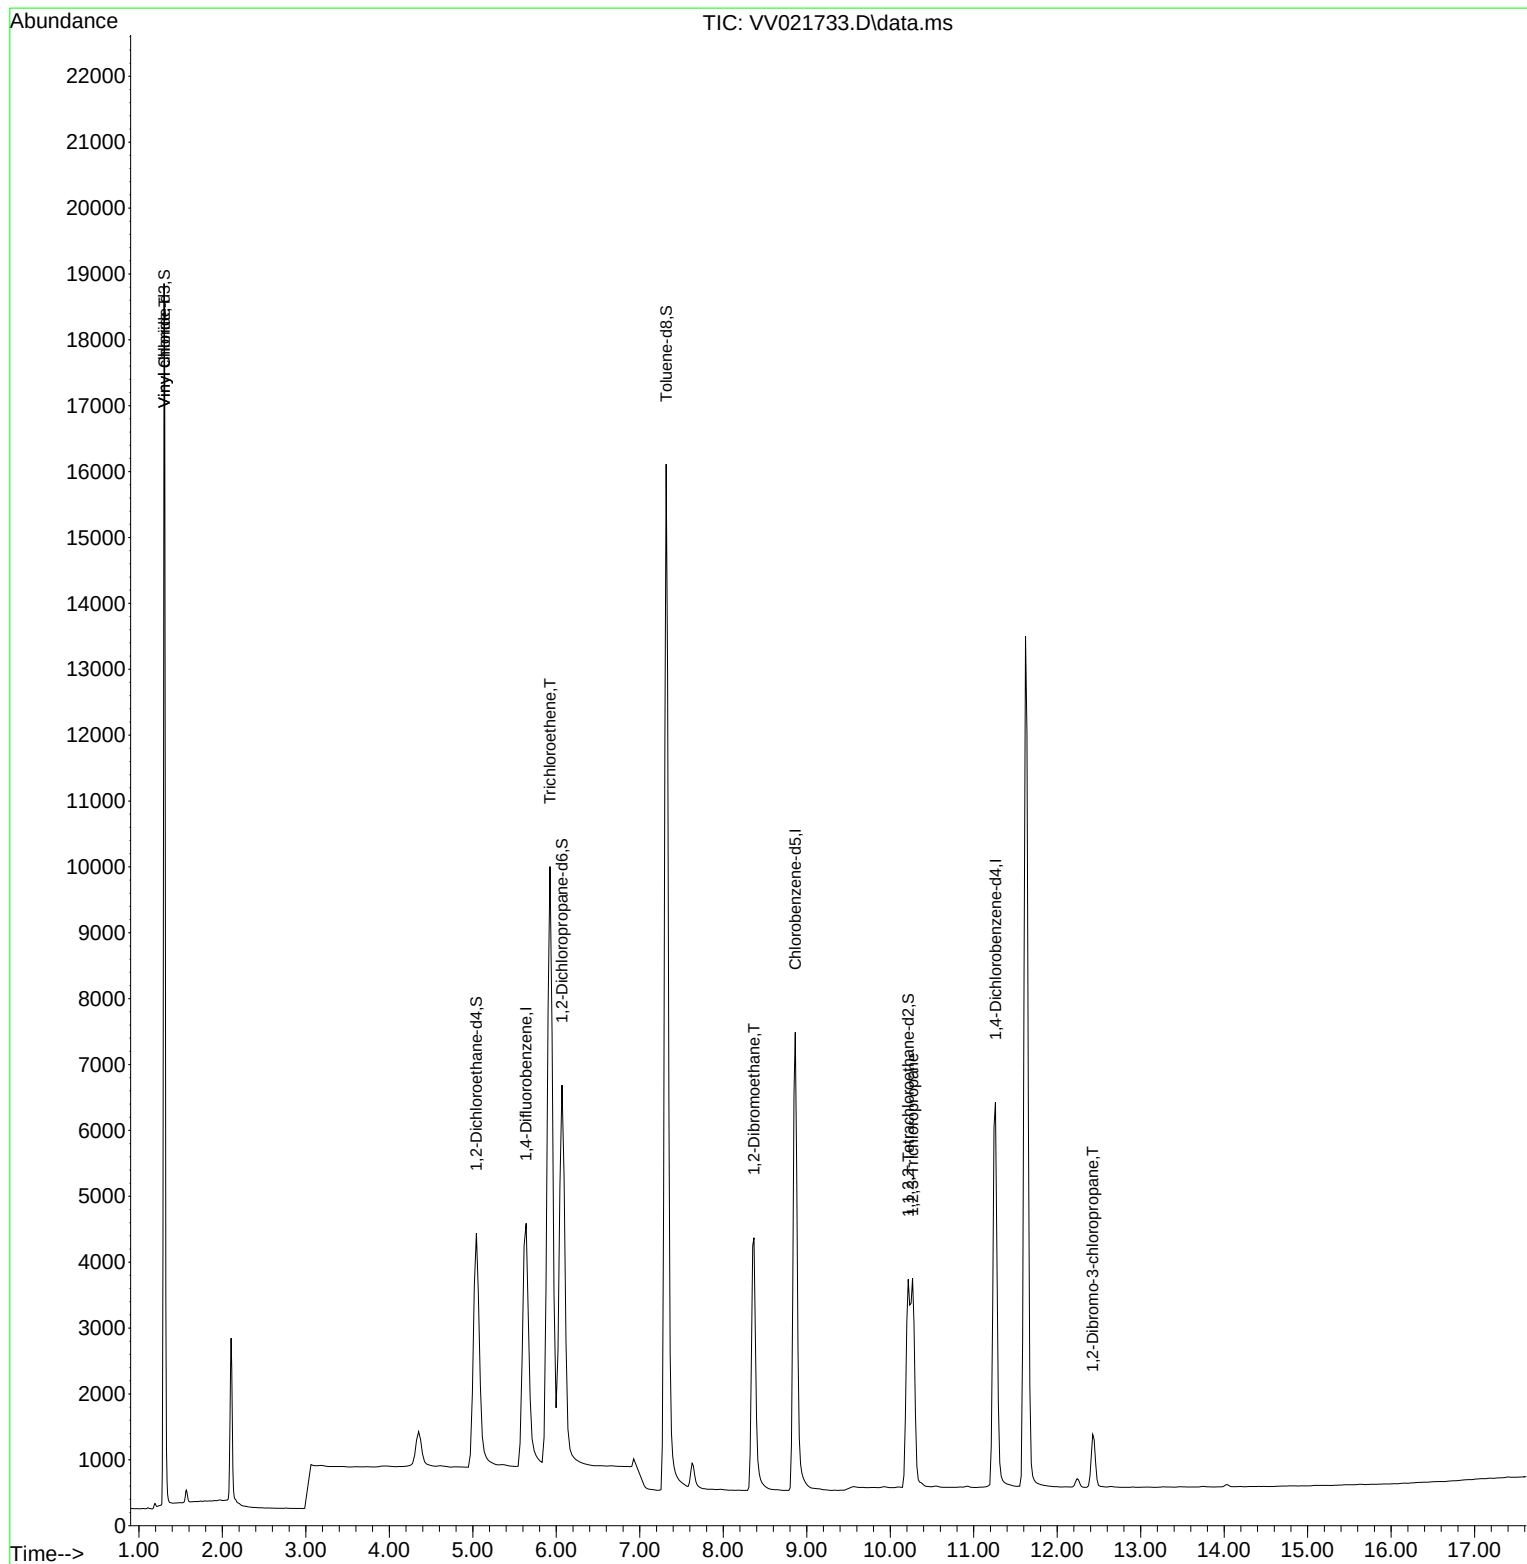

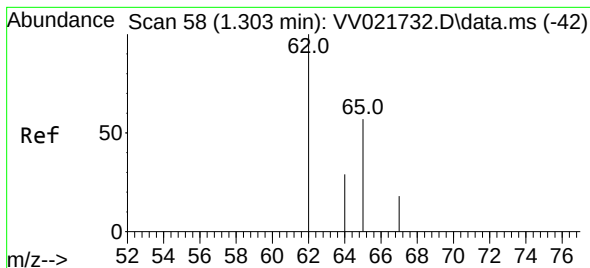

#3

Vinyl chloride

Concen: 1.134 ug/L

RT: 1.303 min Scan# 58

Delta R.T. 0.000 min





Lab File: VV021733.D

Acq: 04 Aug 2021 11:24

Tgt Ion: 62 Resp: 13586

Ion	Ratio	Lower	Upper
62	100		
64	31.2	22.1	41.1

Instrument :
MSVOA_V
ClientSampled :

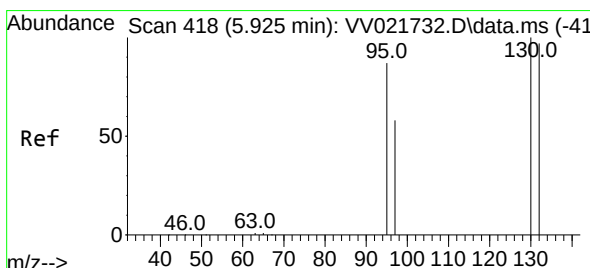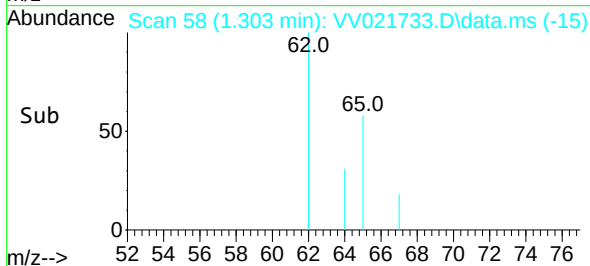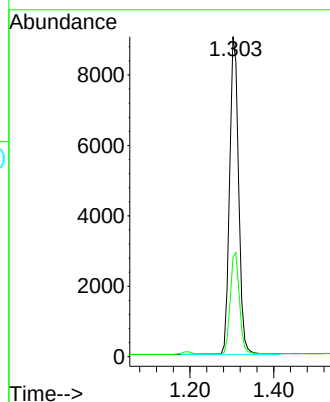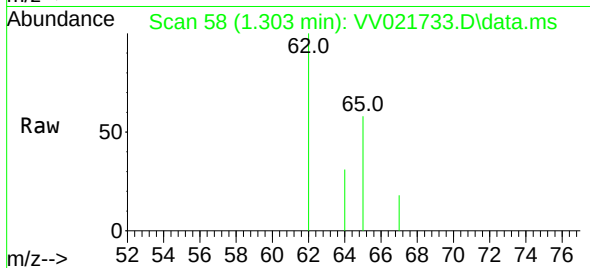

#6

Trichloroethene

Concen: 1.075 ug/L

RT: 5.925 min Scan# 418




Delta R.T. 0.000 min


Lab File: VV021733.D

Acq: 04 Aug 2021 11:24

Tgt Ion: 95 Resp: 11059


Ion	Ratio	Lower	Upper
95	100		
97	66.3	47.3	87.9
132	109.0	76.9	142.7
130	112.0	79.2	147.2

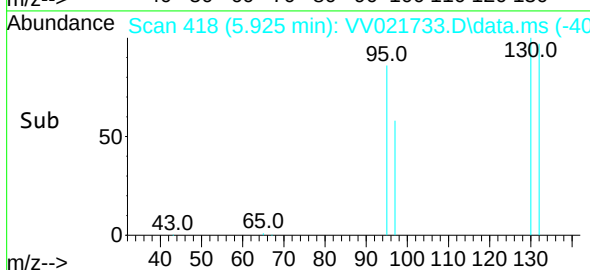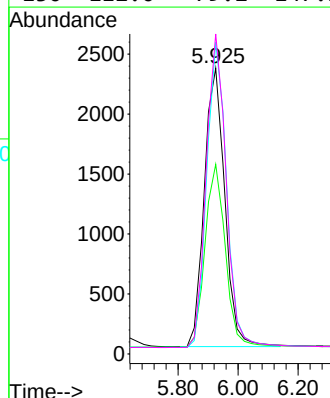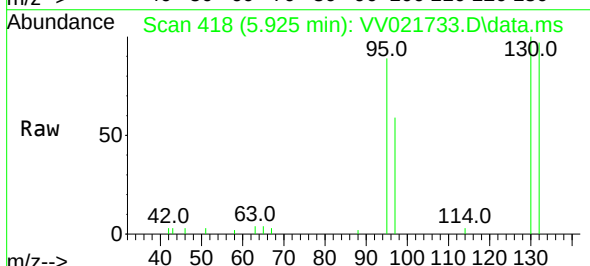



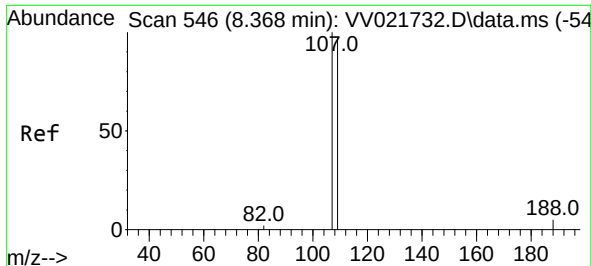


#9
1,2-Dibromoethane
Concen: 1.072 ug/L
RT: 8.368 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV021733.D
Acq: 04 Aug 2021 11:24


Instrument :
MSVOA_V
ClientSampleId :

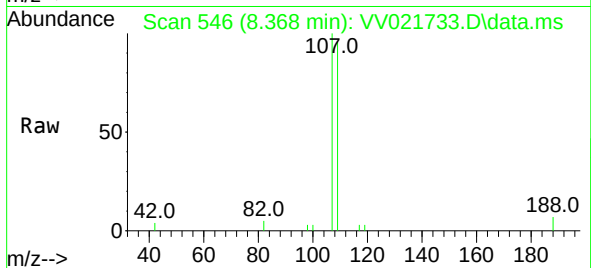



Tgt Ion:107 Resp: 7009
Ion Ratio Lower Upper
107 100
109 96.1 67.7 125.7
188 7.2 7.2 10.8

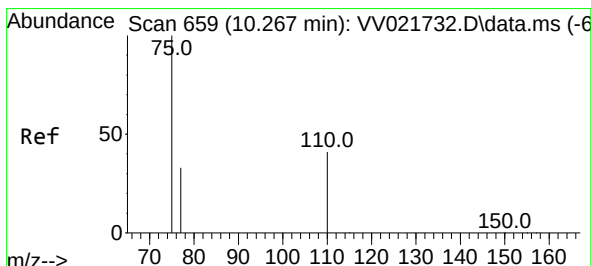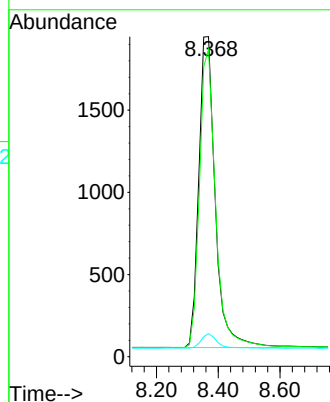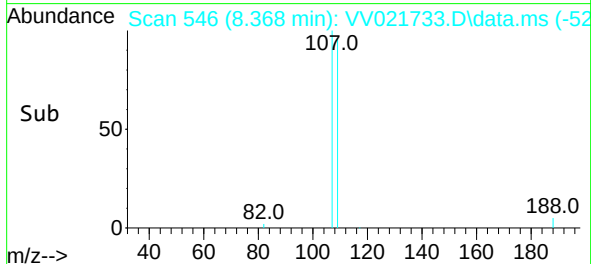


#12
1,2,3-Trichloropropane
Concen: 1.155 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV021733.D
Acq: 04 Aug 2021 11:24

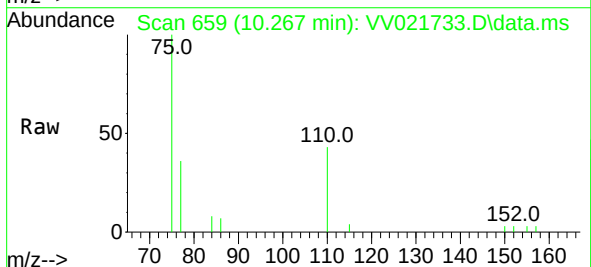


Tgt Ion: 75 Resp: 5819
Ion Ratio Lower Upper
75 100
110 43.8 35.0 52.6
77 33.5 27.0 40.4

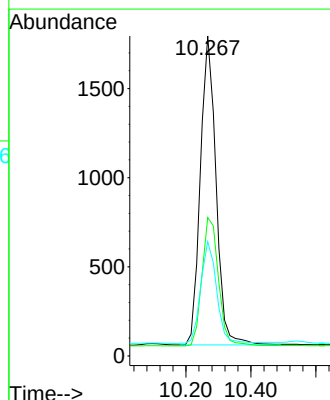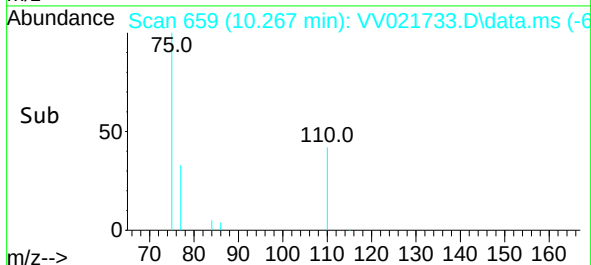

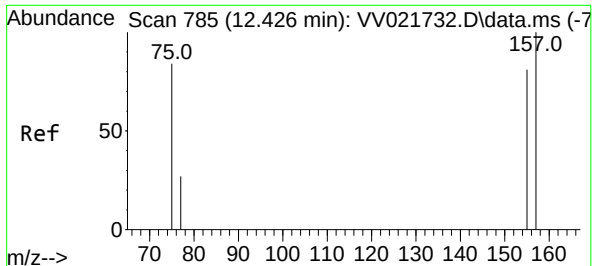

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.978 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV021733.D
 Acq: 04 Aug 2021 11:24

Instrument :
 MSVOA_V
 ClientSampleId :

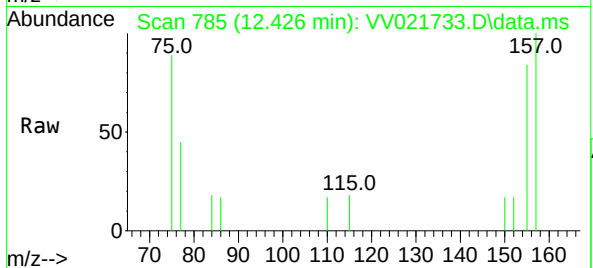

Tgt Ion:	75	Resp:	787
Ion	Ratio	Lower	Upper
75	100		
157	112.3	87.0	130.6
155	94.5	75.0	112.6

