

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080421\
 Data File : VV021736.D
 Acq On : 04 Aug 2021 13:30
 Operator : SY/MD
 Sample : VV0804WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 05 02:40:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Aug 05 02:34:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	13933	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12547	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6210	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	3630	0.508	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.042	65	3631	0.509	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	6.068	67	4923	0.534	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%
8) Toluene-d8	7.317	98	13888	0.523	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2725	0.502	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	100.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.409	75	13	0.017	ug/L	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080421\
Data File : VV021736.D
Acq On : 04 Aug 2021 13:30
Operator : SY/MD
Sample : VV0804WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 05 02:40:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 05 02:34:55 2021
Response via : Initial Calibration

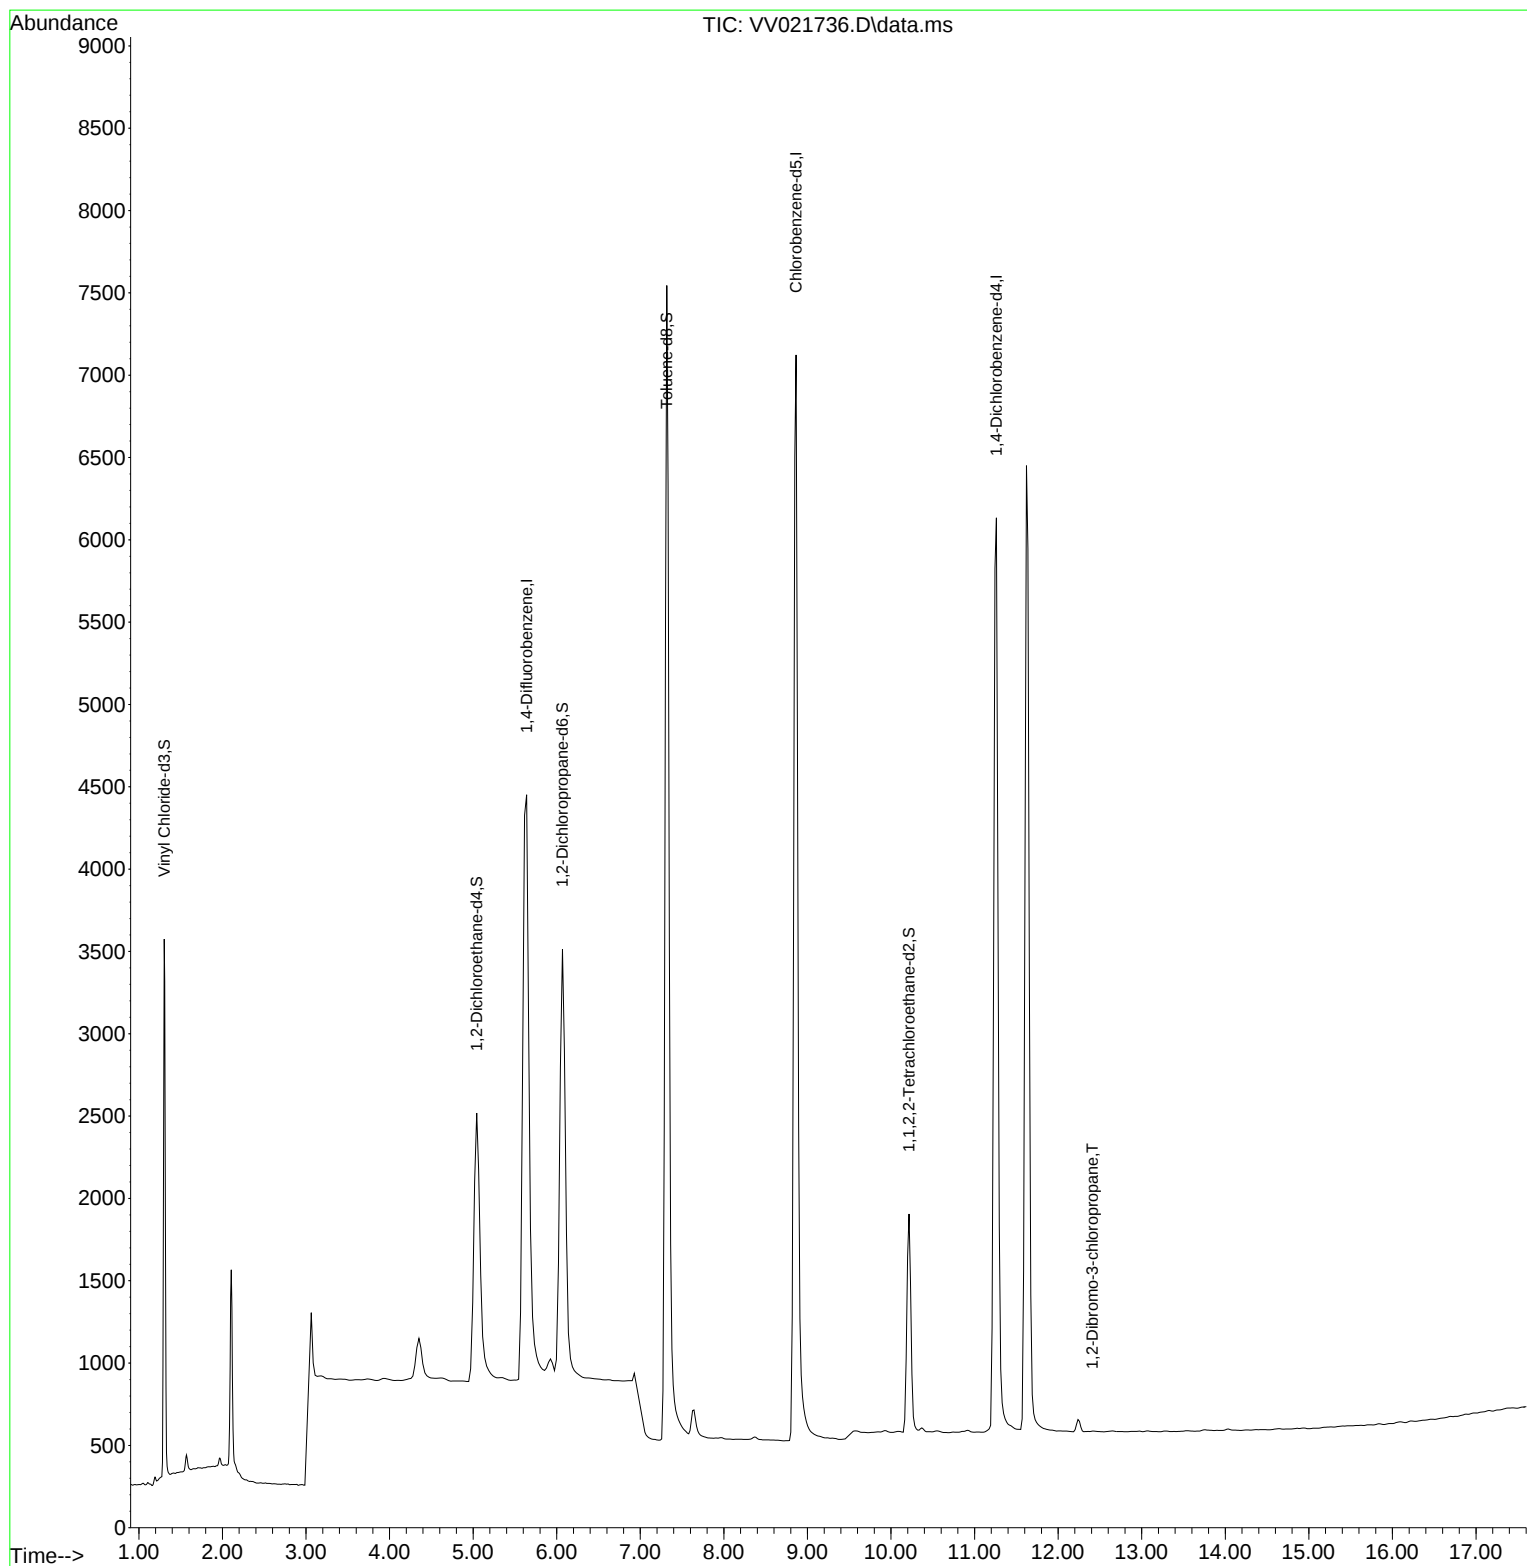

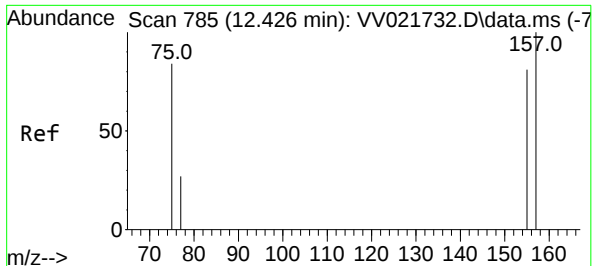

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.017 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. -0.017 min
 Lab File: VV021736.D
 Acq: 04 Aug 2021 13:30

Instrument :
 MSVOA_V
 ClientSampled :

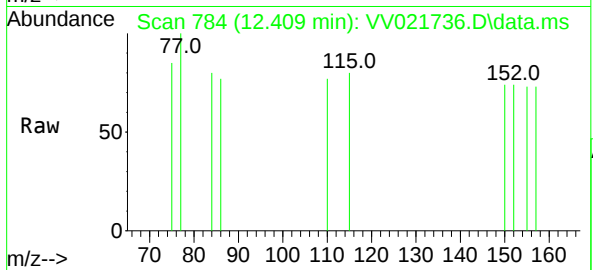

Tgt Ion: 75	Resp: 13
Ion Ratio	Lower Upper
75	100
157	85.7 87.0 130.6#
155	85.7 75.0 112.6

