

m/z	Abundance
39.80	235.0
43.90	453.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	514.0
37.00	2756.0
38.00	2551.0
39.00	1121.0
39.90	241.0
43.90	740.0
44.90	594.0
46.90	862.0
47.90	301.0
49.00	2408.0
50.00	11496.0
51.00	3658.0
51.90	137.0
55.00	197.0
56.00	1160.0
57.00	1740.0
60.00	563.0
61.00	2984.0
62.00	3142.0
63.00	2133.0
64.10	269.0
64.90	233.0
66.90	277.0
68.00	7240.0
69.00	6826.0
70.00	502.0
70.80	115.0
72.00	294.0
73.00	2933.0
74.00	11631.0
75.00	33592.0
76.00	2937.0
77.00	451.0
78.00	413.0
78.90	2085.0
79.90	675.0
80.90	2070.0
81.90	465.0
86.90	2796.0
87.90	3358.0
91.00	298.0
92.00	1992.0
93.00	3072.0
94.00	8587.0
95.00	70480.0
96.00	4564.0
97.00	187.0
103.80	257.0
104.80	173.0
105.90	342.0
115.90	274.0
116.90	533.0
117.80	289.0
118.90	454.0
127.90	254.0
128.80	106.0
129.90	231.0
130.90	163.0
134.90	149.0
137.00	150.0
140.90	714.0
142.90	825.0
145.80	191.0
148.00	139.0
154.00	107.0
154.80	185.0
157.00	141.0
158.80	112.0
171.80	314.0
173.00	520.0
173.90	62520.0
175.00	4409.0
175.90	60368.0
177.00	3753.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	531.0
37.00	3077.0
38.00	2777.0
39.00	1269.0
40.00	221.0
43.90	830.0
44.90	743.0
46.00	103.0
46.90	851.0
47.90	319.0
49.00	2740.0
50.00	12119.0
51.00	3863.0
51.90	154.0
55.00	206.0
56.00	1124.0
57.00	1859.0
60.00	583.0
61.00	3035.0
62.00	3231.0
63.00	2183.0
64.00	246.0
64.90	281.0
66.90	274.0
68.00	7701.0
69.00	7284.0
69.90	540.0
71.90	398.0
73.00	3138.0
74.00	12449.0
75.00	36048.0
76.00	3120.0
77.10	532.0
78.00	377.0
78.90	2201.0
79.90	681.0
80.90	2240.0
81.90	529.0
86.00	117.0
86.90	3104.0
87.90	3366.0
90.90	310.0
92.00	2196.0
93.00	3159.0
94.00	8889.0
95.00	74400.0
96.00	4971.0
97.10	210.0
103.80	229.0
104.70	161.0
105.90	406.0
106.80	122.0
115.70	260.0
116.90	488.0
117.80	266.0
118.90	418.0
127.90	249.0
129.00	118.0
129.80	245.0
130.90	128.0
134.90	149.0
137.00	171.0
140.90	764.0
142.90	888.0
145.80	202.0
147.80	175.0
149.90	105.0
154.90	207.0
156.80	123.0
161.00	103.0
171.90	332.0
172.90	576.0
173.90	63456.0
175.00	4461.0
175.90	61152.0
177.00	4086.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	496.0
37.00	3084.0
38.00	2641.0
39.00	1213.0
40.00	197.0
43.90	873.0
44.90	764.0
46.00	105.0
47.00	783.0
47.90	336.0
49.00	2669.0
50.00	11792.0
51.00	3820.0
51.90	155.0
55.00	198.0
56.00	1083.0
57.00	1838.0
60.00	559.0
61.00	2882.0
62.00	3088.0
63.00	2214.0
63.90	222.0
64.90	266.0
66.90	240.0
68.00	7182.0
69.00	6982.0
70.00	574.0
71.90	466.0
73.00	2994.0
74.00	12098.0
75.00	34848.0
76.00	3175.0
77.10	534.0
78.00	292.0
79.00	2153.0
79.90	604.0
80.90	2231.0
81.90	507.0
86.00	116.0
86.90	3169.0
87.90	2981.0
90.90	312.0
92.00	2032.0
93.00	3026.0
94.00	8443.0
95.00	71400.0
96.00	4806.0
97.00	192.0
103.70	221.0
103.90	218.0
104.70	130.0
105.80	426.0
106.80	139.0
110.80	137.0
111.80	123.0
114.80	119.0
115.70	234.0
116.90	420.0
117.80	232.0
118.90	392.0
127.90	255.0
129.00	104.0
129.80	246.0
134.90	134.0
136.90	163.0
140.90	746.0
142.90	877.0
145.70	160.0
146.80	102.0
147.80	167.0
154.90	210.0
157.10	106.0
161.00	111.0
171.90	326.0
172.90	587.0
173.90	58392.0
175.00	4201.0
175.90	56256.0
177.00	3793.0



Instrument :
MSVOA_V
ClientSampleId :
BFB202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080421\
 Data File : VV021729.D
 Acq On : 04 Aug 2021 09:04
 Operator : SY/MD
 Sample : BFB202
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB202

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 06 01:25:29 2021

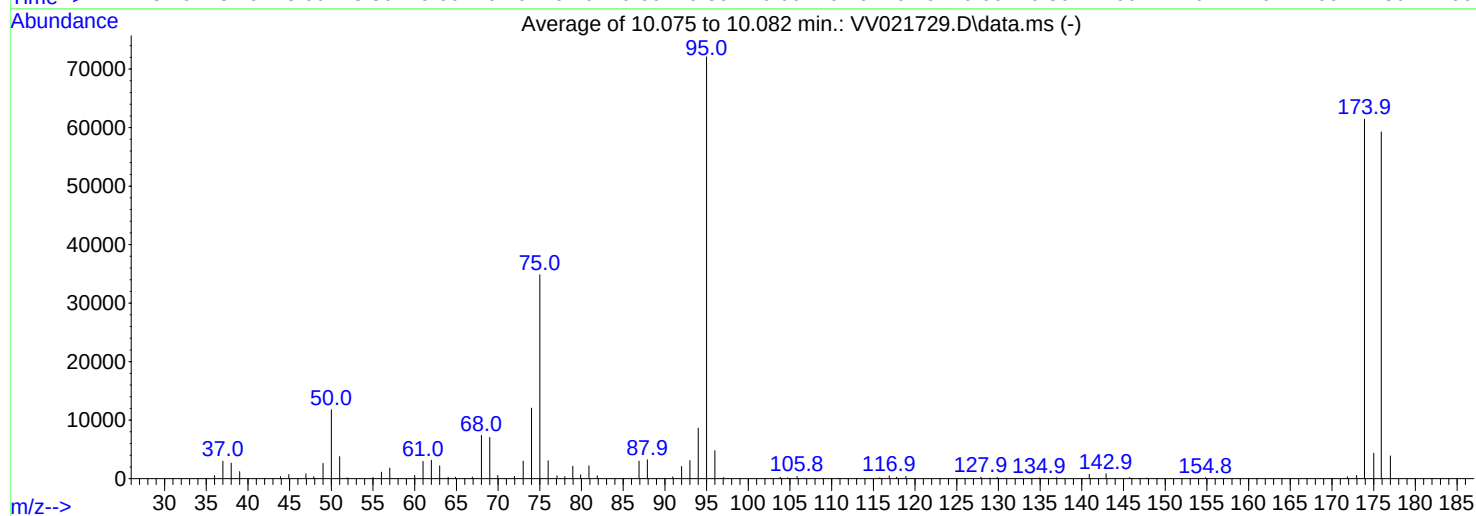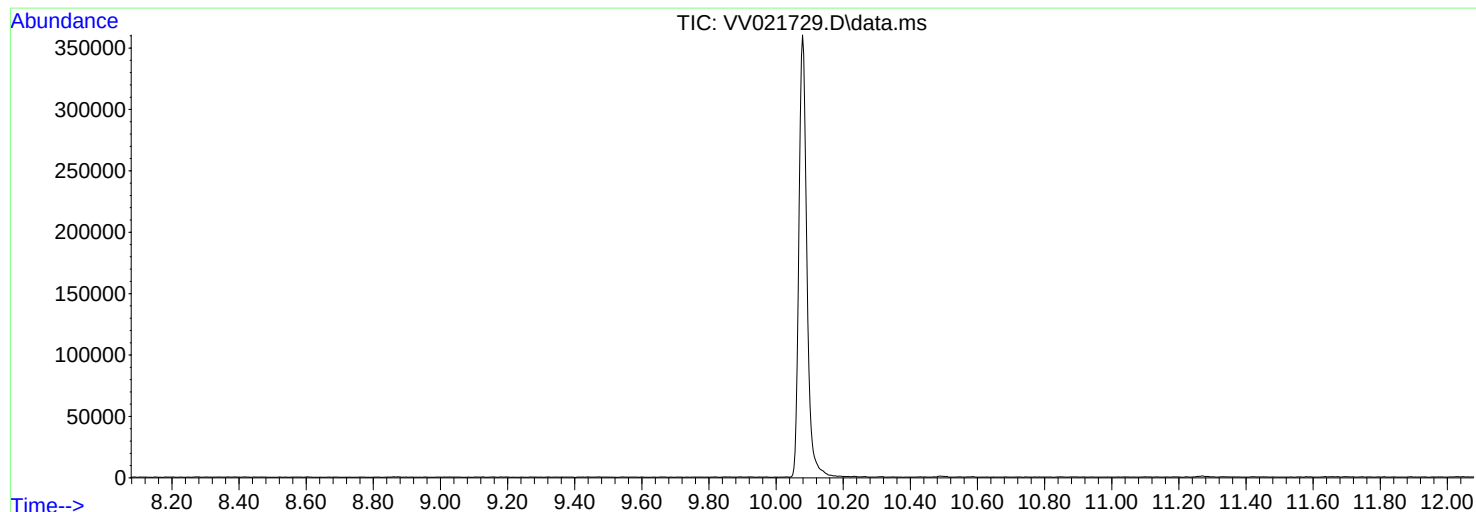

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11802	PASS
75	95	30	80	48.3	34829	PASS
95	95	100	100	100.0	72093	PASS
96	95	5	9	6.6	4780	PASS
173	174	0.00	2	0.9	561	PASS
174	95	50	120	85.2	61456	PASS
175	174	5	9	7.1	4357	PASS
176	174	95	101	96.4	59259	PASS
177	176	5	9	6.5	3877	PASS