

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027213.D
 Acq On : 04 Aug 2022 17:02
 Operator : SY/MD
 Sample : VV0804WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Quant Time: Aug 05 02:30:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 05 02:29:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	350561	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	8.850	117	344783	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	142601	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	144714	60.549	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	121.100%	
7) Chloroethane-d5	1.561	69	110731	63.374	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	126.740%	
11) 1,1-Dichloroethene-d2	2.101	63	186646	42.694	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.380%	
21) 2-Butanone-d5	3.870	46	182668	85.863	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	85.860%	
24) Chloroform-d	4.342	84	249599	50.983	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.960%	
26) 1,2-Dichloroethane-d4	5.027	65	159914	52.609	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.220%	
32) Benzene-d6	5.043	84	485596	58.731	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	117.460%	
36) 1,2-Dichloropropane-d6	6.066	67	161711	54.983	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	109.960%	
41) Toluene-d8	7.313	98	398631	56.563	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.120%	
43) trans-1,3-Dichloroprop...	7.619	79	65570	51.148	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	102.300%	
47) 2-Hexanone-d5	8.085	63	117474	82.929	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	82.930%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	209597	43.730	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.460%	
66) 1,2-Dichlorobenzene-d4	11.622	152	139493	56.645	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.280%	
Target Compounds						
27) 1,2-Dichloroethane	5.040	62	3373	0.794	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027213.D
Acq On : 04 Aug 2022 17:02
Operator : SY/MD
Sample : VV0804WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Time: Aug 05 02:30:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 05 02:29:34 2022
Response via : Initial Calibration

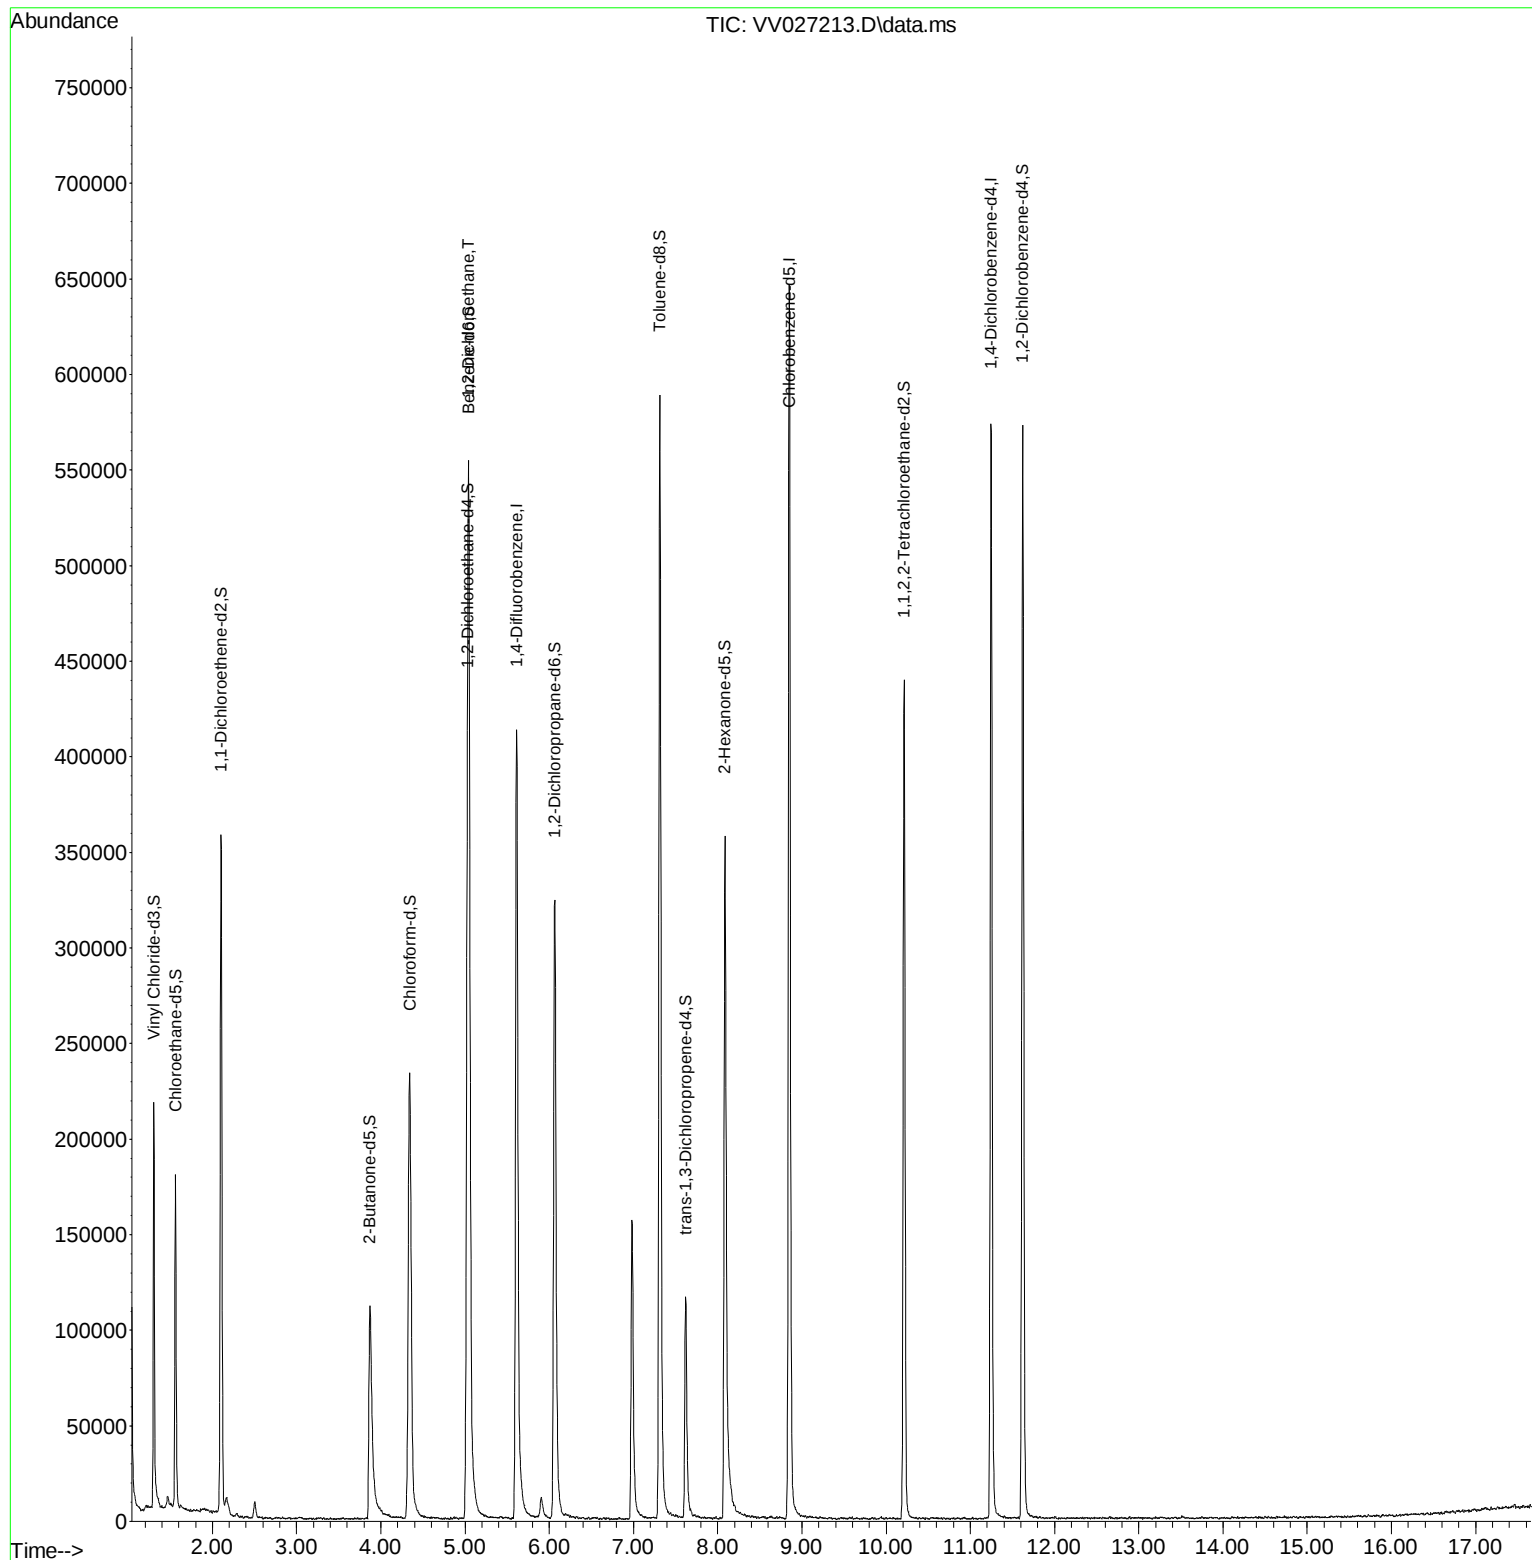

Abundance Scan 1269 (5.120 min): VV027211.D\data.ms (-12517)

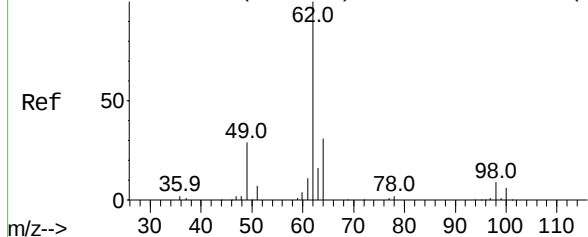

1,2-Dichloroethane

Concen: 0.794 ug/L

RT: 5.040 min Scan# 1

Delta R.T. -0.080 min

Lab File: VV027213.D

Acq: 04 Aug 2022 17:02

Instrument :

MSVOA_V

ClientSampleId :



VBLK251

Tgt Ion: 62 Resp: 3373

Ion Ratio Lower Upper

62 100

98 12.9 9.0 13.6

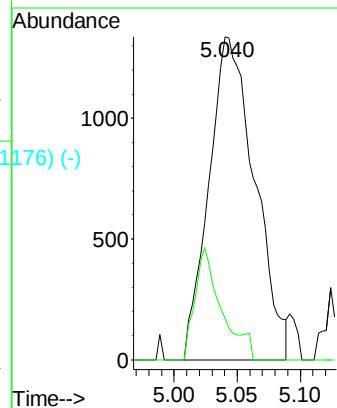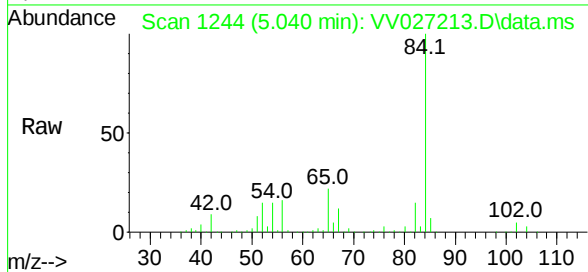

Abundance Scan 1244 (5.040 min): VV027213.D\data.ms (-1176) (-)

