

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027213.D
 Acq On : 04 Aug 2022 17:02
 Operator : SY/MD
 Sample : VV0804WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	105	rBV	211807	231444	15.76%	2.149%
2	1.561	155	162	177	rVB	174429	201499	13.72%	1.871%
3	2.101	321	330	343	rBV	353024	496818	33.82%	4.613%
4	2.503	447	455	467	rVB3	8593	14389	0.98%	0.134%
5	2.732	522	526	527	rBV2	496	380	0.03%	0.004%
6	2.941	588	591	592	rBV	572	307	0.02%	0.003%
7	3.121	644	647	649	rBV2	618	306	0.02%	0.003%
8	3.240	682	684	687	rBV3	747	370	0.03%	0.003%
9	3.262	687	691	694	rBV4	735	626	0.04%	0.006%
10	3.365	721	723	725	rVB	788	317	0.02%	0.003%
11	3.400	732	734	739	rVB2	834	608	0.04%	0.006%
12	3.449	745	749	750	rBV2	547	346	0.02%	0.003%
13	3.478	755	758	760	rBV3	619	347	0.02%	0.003%
14	3.535	773	776	778	rVV3	567	375	0.03%	0.003%
15	3.555	780	782	784	rVB3	758	287	0.02%	0.003%
16	3.648	809	811	814	rBV	573	322	0.02%	0.003%
17	3.722	832	834	839	rVB5	737	470	0.03%	0.004%
18	3.870	871	880	914	rBV	111601	314506	21.41%	2.920%
19	4.342	1012	1027	1062	rBV	232093	586639	39.94%	5.447%
20	4.741	1149	1151	1153	rBV	519	285	0.02%	0.003%
21	4.767	1155	1159	1163	rBV4	814	661	0.05%	0.006%
22	4.828	1175	1178	1183	rBV5	1180	934	0.06%	0.009%
23	4.867	1187	1190	1194	rVV5	870	707	0.05%	0.007%
24	4.937	1208	1212	1216	rBV5	928	847	0.06%	0.008%
25	5.040	1228	1244	1282	rBV2	553240	1468827	100.00%	13.639%
26	5.561	1402	1406	1407	rBV2	840	547	0.04%	0.005%
27	5.613	1410	1422	1454	rBV	412874	873280	59.45%	8.109%
28	6.066	1546	1563	1592	rBV	323564	689780	46.96%	6.405%
29	6.352	1650	1652	1653	rBV2	500	260	0.02%	0.002%
30	6.567	1718	1719	1726	rVB4	1262	756	0.05%	0.007%
31	6.600	1726	1729	1732	rBV3	575	479	0.03%	0.004%
32	6.641	1737	1742	1743	rBV3	912	643	0.04%	0.006%
33	6.677	1751	1753	1755	rBV3	861	416	0.03%	0.004%
34	6.738	1766	1772	1774	rBV6	770	686	0.05%	0.006%
35	6.764	1776	1780	1782	rBV2	528	466	0.03%	0.004%
36	6.805	1791	1793	1796	rBV3	740	399	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027213.D
 Acq On : 04 Aug 2022 17:02
 Operator : SY/MD
 Sample : VV0804WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.828	1796	1800	1803	rBV3	772	675	0.05%	0.006%
38	6.866	1810	1812	1817	rVB4	644	468	0.03%	0.004%
39	6.892	1817	1820	1821	rBV3	570	326	0.02%	0.003%
40	6.912	1824	1826	1830	rBV4	667	446	0.03%	0.004%
41	6.982	1837	1848	1872	rBV	156590	299743	20.41%	2.783%
42	7.313	1939	1951	1980	rBV	587800	1072099	72.99%	9.955%
43	7.619	2037	2046	2063	rBV	115135	202873	13.81%	1.884%
44	7.838	2112	2114	2117	rBV4	870	666	0.05%	0.006%
45	7.931	2141	2143	2146	rVB2	865	403	0.03%	0.004%
46	7.953	2146	2150	2152	rBV4	883	671	0.05%	0.006%
47	7.979	2154	2158	2163	rVB4	1553	1172	0.08%	0.011%
48	8.021	2169	2171	2172	rBV4	759	375	0.03%	0.003%
49	8.085	2182	2191	2224	rBV	356495	703728	47.91%	6.534%
50	8.561	2337	2339	2344	rVB4	1348	904	0.06%	0.008%
51	8.583	2344	2346	2347	rBV	826	426	0.03%	0.004%
52	8.600	2349	2351	2354	rBV3	746	547	0.04%	0.005%
53	8.850	2417	2429	2459	rVV	645662	1073461	73.08%	9.968%
54	9.214	2537	2542	2547	rBV6	1265	1464	0.10%	0.014%
55	9.320	2571	2575	2578	rBV4	822	710	0.05%	0.007%
56	9.429	2605	2609	2610	rBV2	886	521	0.04%	0.005%
57	9.500	2627	2631	2633	rBV4	723	521	0.04%	0.005%
58	9.545	2643	2645	2649	rBV4	683	473	0.03%	0.004%
59	9.571	2649	2653	2655	rBV4	1081	779	0.05%	0.007%
60	9.696	2689	2692	2693	rBV2	517	291	0.02%	0.003%
61	9.754	2708	2710	2713	rVB2	571	335	0.02%	0.003%
62	9.924	2760	2763	2764	rBV	476	279	0.02%	0.003%
63	10.214	2839	2853	2874	rBV	439053	695974	47.38%	6.462%
64	10.471	2931	2933	2940	rBV5	1051	1145	0.08%	0.011%
65	10.532	2947	2952	2954	rBV5	798	787	0.05%	0.007%
66	10.599	2971	2973	2977	rVB2	746	451	0.03%	0.004%
67	10.683	2995	2999	3004	rBV4	763	693	0.05%	0.006%
68	10.715	3006	3009	3010	rBV3	619	304	0.02%	0.003%
69	10.738	3014	3016	3020	rVB2	728	510	0.03%	0.005%
70	10.767	3020	3025	3026	rBV2	815	425	0.03%	0.004%
71	10.908	3066	3069	3070	rBV2	474	290	0.02%	0.003%
72	10.985	3091	3093	3096	rVB2	666	317	0.02%	0.003%
73	11.017	3100	3103	3104	rVV2	645	353	0.02%	0.003%
74	11.027	3104	3106	3108	rVB3	1107	432	0.03%	0.004%
75	11.091	3123	3126	3128	rBV2	512	275	0.02%	0.003%
76	11.246	3163	3174	3193	rBV	572457	892001	60.73%	8.283%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027213.D
 Acq On : 04 Aug 2022 17:02
 Operator : SY/MD
 Sample : VV0804WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

77	11.493	3248	3251	3252	rBV2	788	477	0.03%	0.004%
78	11.622	3279	3291	3311	rBV	571874	907853	61.81%	8.430%
79	12.146	3450	3454	3456	rBV4	705	533	0.04%	0.005%
80	12.300	3501	3502	3504	rBV2	559	279	0.02%	0.003%
81	12.355	3517	3519	3521	rBV3	759	394	0.03%	0.004%
82	12.477	3554	3557	3560	rBV2	799	484	0.03%	0.004%
83	12.570	3582	3586	3591	rBV5	1103	1117	0.08%	0.010%
84	12.648	3607	3610	3611	rBV4	1073	577	0.04%	0.005%
85	12.673	3616	3618	3623	rVB4	781	523	0.04%	0.005%
86	12.718	3630	3632	3638	rVB3	762	650	0.04%	0.006%
87	12.747	3639	3641	3645	rVB4	696	356	0.02%	0.003%
88	12.889	3679	3685	3689	rBV4	1039	1106	0.08%	0.010%
89	13.053	3734	3736	3737	rBV2	741	274	0.02%	0.003%
90	13.172	3770	3773	3775	rBV2	852	398	0.03%	0.004%
91	13.259	3795	3800	3801	rBV3	970	814	0.06%	0.008%
92	13.387	3836	3840	3842	rBV4	694	556	0.04%	0.005%
93	13.963	4017	4019	4020	rBV	883	399	0.03%	0.004%
94	14.082	4054	4056	4059	rBV2	438	273	0.02%	0.003%
95	14.107	4062	4064	4067	rVB3	925	445	0.03%	0.004%
96	14.262	4110	4112	4116	rBV4	893	750	0.05%	0.007%
97	14.426	4160	4163	4164	rBV	1071	544	0.04%	0.005%
98	14.570	4206	4208	4212	rVB5	922	558	0.04%	0.005%
99	14.635	4225	4228	4230	rBV5	1266	818	0.06%	0.008%
100	14.979	4332	4335	4337	rBV4	897	634	0.04%	0.006%




Sum of corrected areas: 10769454

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027213.D
Acq On : 04 Aug 2022 17:02
Operator : SY/MD
Sample : VV0804WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

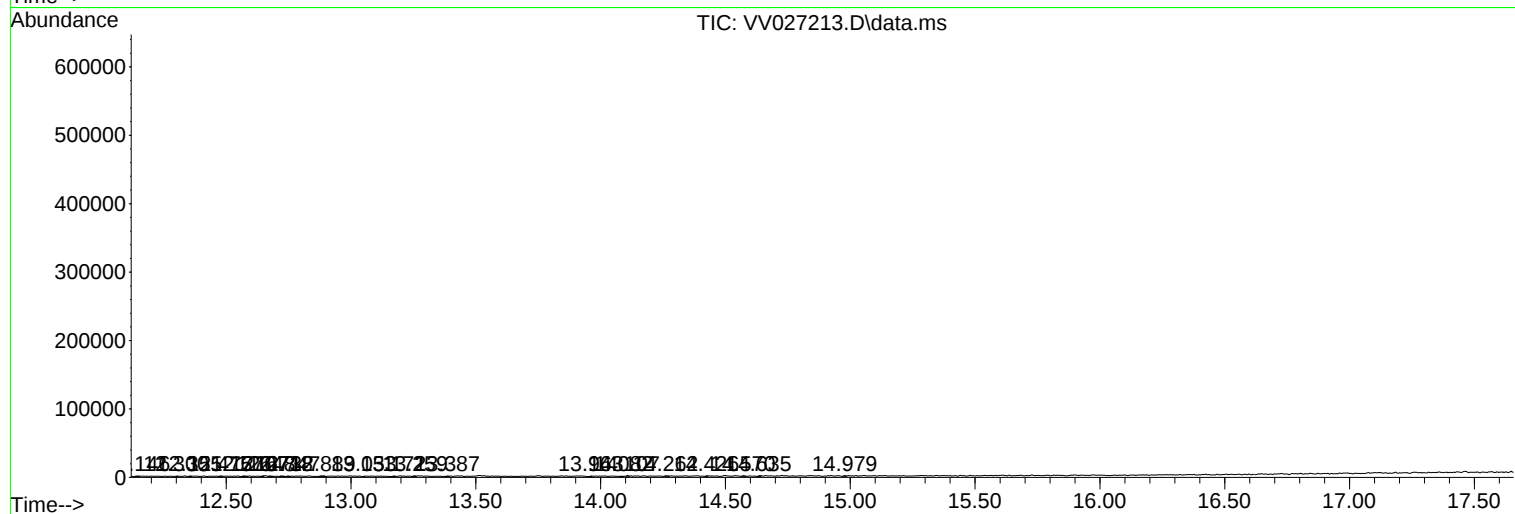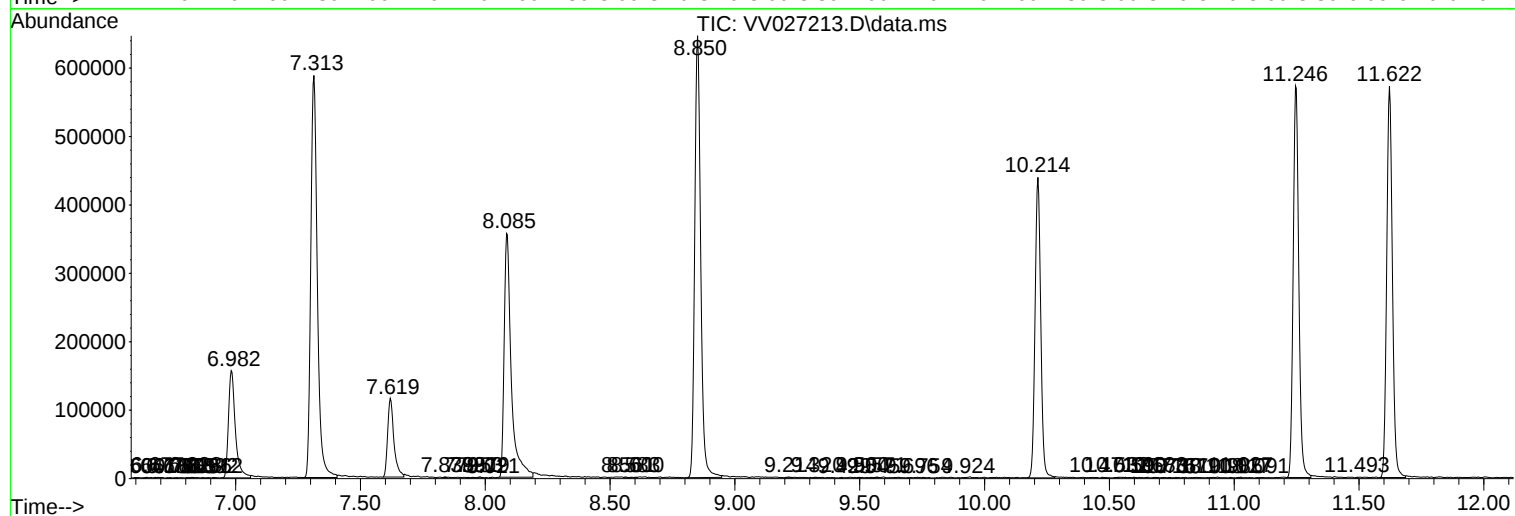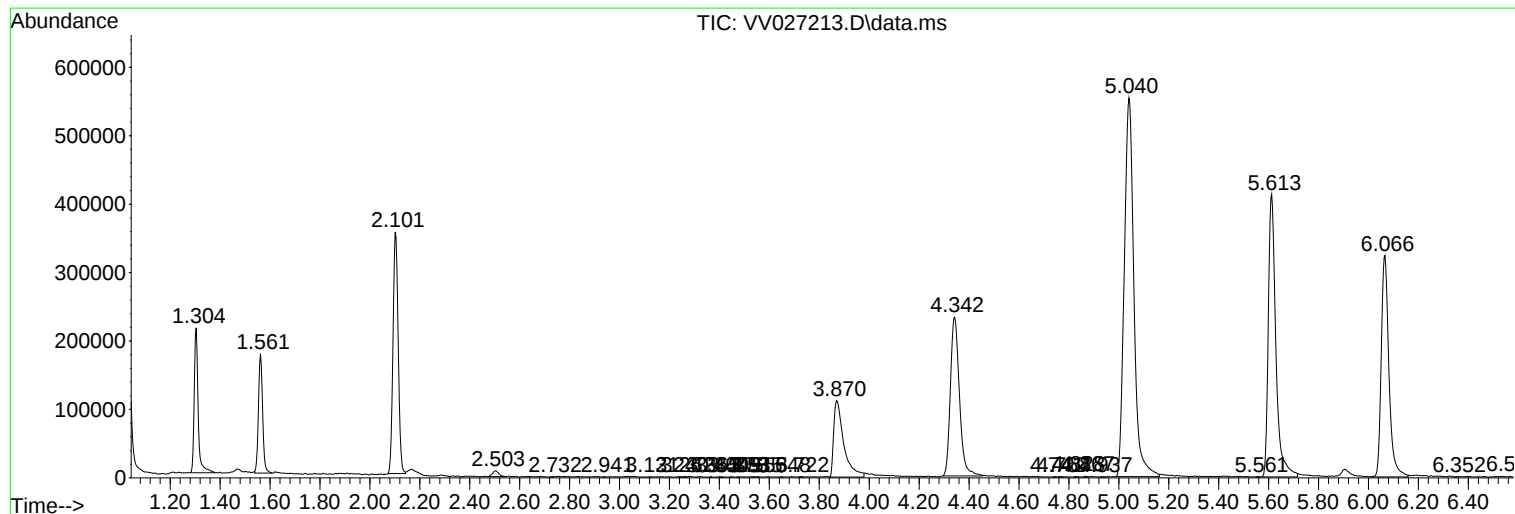

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027213.D
Acq On : 04 Aug 2022 17:02
Operator : SY/MD
Sample : VV0804WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027213.D
Acq On : 04 Aug 2022 17:02
Operator : SY/MD
Sample : VV0804WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc