

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027214.D
 Acq On : 04 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	109	rBV	325284	363352	15.94%	2.418%
2	1.561	155	162	174	rVB	258528	300758	13.19%	2.002%
3	2.101	320	330	342	rBV	551831	777718	34.11%	5.176%
4	2.500	446	454	468	rVB2	12544	22726	1.00%	0.151%
5	2.564	472	474	478	rVB3	960	656	0.03%	0.004%
6	2.616	487	490	493	rBV3	639	473	0.02%	0.003%
7	2.696	511	515	517	rVB4	660	404	0.02%	0.003%
8	2.751	519	532	548	rBV	533456	920111	40.36%	6.124%
9	3.002	608	610	615	rVB4	1070	560	0.02%	0.004%
10	3.034	615	620	622	rBV3	1461	1411	0.06%	0.009%
11	3.108	641	643	650	rBV4	678	559	0.02%	0.004%
12	3.211	673	675	679	rBV3	461	278	0.01%	0.002%
13	3.285	696	698	700	rBV3	782	325	0.01%	0.002%
14	3.294	700	701	704	rVB2	641	268	0.01%	0.002%
15	3.323	706	710	713	rBV3	537	501	0.02%	0.003%
16	3.339	713	715	716	rBV	641	274	0.01%	0.002%
17	3.513	767	769	772	rBV3	682	438	0.02%	0.003%
18	3.587	789	792	794	rVB	715	397	0.02%	0.003%
19	3.606	794	798	801	rBV4	959	701	0.03%	0.005%
20	3.622	801	803	805	rVB	528	262	0.01%	0.002%
21	3.648	805	811	812	rBV3	660	624	0.03%	0.004%
22	3.696	822	826	829	rBV4	710	570	0.02%	0.004%
23	3.748	840	842	846	rVB2	707	370	0.02%	0.002%
24	3.783	851	853	854	rBV2	625	281	0.01%	0.002%
25	3.815	860	863	864	rBV3	880	349	0.02%	0.002%
26	3.895	868	888	914	rBV3	262473	1016418	44.58%	6.765%
27	4.336	1010	1025	1057	rBV	358622	903489	39.63%	6.013%
28	4.632	1115	1117	1120	rBV3	651	389	0.02%	0.003%
29	4.760	1153	1157	1158	rBV3	606	422	0.02%	0.003%
30	4.854	1183	1186	1187	rBV	478	259	0.01%	0.002%
31	4.879	1192	1194	1196	rVV2	740	267	0.01%	0.002%
32	4.915	1203	1205	1206	rBV	919	429	0.02%	0.003%
33	5.037	1226	1243	1291	rVV2	867862	2280025	100.00%	15.175%
34	5.535	1395	1398	1399	rBV3	595	340	0.01%	0.002%
35	5.609	1410	1421	1453	rBV	183657	398695	17.49%	2.654%
36	5.908	1503	1514	1540	rVB8	34324	82451	3.62%	0.549%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027214.D
 Acq On : 04 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.059	1545	1561	1593	rBV	501549	1052289	46.15%	7.004%
38	6.355	1651	1653	1655	rBV2	853	403	0.02%	0.003%
39	6.432	1675	1677	1680	rVB3	896	363	0.02%	0.002%
40	6.461	1680	1686	1689	rBV5	930	1082	0.05%	0.007%
41	6.500	1696	1698	1701	rVB4	957	419	0.02%	0.003%
42	6.571	1718	1720	1721	rBV2	608	291	0.01%	0.002%
43	6.712	1762	1764	1766	rBV3	746	359	0.02%	0.002%
44	6.728	1766	1769	1773	rVV4	757	564	0.02%	0.004%
45	6.757	1775	1778	1779	rVV	635	376	0.02%	0.003%
46	6.776	1782	1784	1786	rVV2	951	514	0.02%	0.003%
47	6.789	1786	1788	1789	rVV2	568	253	0.01%	0.002%
48	6.863	1805	1811	1814	rBV6	801	552	0.02%	0.004%
49	6.979	1836	1847	1870	rBV	248875	460536	20.20%	3.065%
50	7.169	1904	1906	1908	rBV3	896	524	0.02%	0.003%
51	7.310	1938	1950	1976	rBV	978277	1714040	75.18%	11.408%
52	7.616	2035	2045	2063	rBV	181828	318873	13.99%	2.122%
53	7.899	2130	2133	2139	rBV5	1068	1036	0.05%	0.007%
54	8.082	2180	2190	2230	rBV	577273	1099736	48.23%	7.319%
55	8.603	2349	2352	2354	rBV5	828	490	0.02%	0.003%
56	8.847	2418	2428	2453	rBV	284446	486848	21.35%	3.240%
57	9.069	2493	2497	2499	rBV3	1104	1095	0.05%	0.007%
58	9.217	2542	2543	2547	rVB2	674	365	0.02%	0.002%
59	9.239	2547	2550	2551	rBV3	665	347	0.02%	0.002%
60	9.291	2562	2566	2567	rBV3	563	421	0.02%	0.003%
61	9.329	2574	2578	2579	rBV2	563	408	0.02%	0.003%
62	9.403	2599	2601	2602	rBV2	618	283	0.01%	0.002%
63	9.461	2616	2619	2621	rBV3	720	498	0.02%	0.003%
64	9.567	2649	2652	2653	rBV3	562	318	0.01%	0.002%
65	9.648	2674	2677	2679	rBV2	684	412	0.02%	0.003%
66	9.757	2708	2711	2714	rBV3	1029	687	0.03%	0.005%
67	9.841	2732	2737	2740	rBV5	666	685	0.03%	0.005%
68	9.979	2776	2780	2781	rBV2	478	361	0.02%	0.002%
69	10.117	2820	2823	2827	rBV5	644	468	0.02%	0.003%
70	10.210	2836	2852	2878	rBV	655645	1051623	46.12%	6.999%
71	10.419	2914	2917	2919	rBV2	553	377	0.02%	0.003%
72	10.439	2919	2923	2925	rVV2	697	517	0.02%	0.003%
73	10.455	2925	2928	2933	rVB3	796	612	0.03%	0.004%
74	10.522	2947	2949	2951	rBV2	571	278	0.01%	0.002%
75	10.847	3045	3050	3052	rBV4	1023	872	0.04%	0.006%
76	11.107	3127	3131	3134	rVB2	360	281	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
 Data File : VV027214.D
 Acq On : 04 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.152	3141	3145	3146	rBV4	529	357	0.02%	0.002%
78	11.246	3163	3174	3192	rBV	244324	389365	17.08%	2.591%
79	11.429	3229	3231	3233	rBV3	655	316	0.01%	0.002%
80	11.622	3278	3291	3310	rBV	858267	1346993	59.08%	8.965%
81	12.133	3449	3450	3452	rBV2	763	357	0.02%	0.002%
82	12.271	3490	3493	3494	rBV	707	355	0.02%	0.002%
83	12.300	3500	3502	3505	rBV3	620	328	0.01%	0.002%
84	12.651	3607	3611	3613	rBV3	852	568	0.02%	0.004%
85	12.667	3613	3616	3618	rVB2	958	531	0.02%	0.004%
86	12.889	3681	3685	3689	rBV4	1099	1234	0.05%	0.008%
87	12.908	3689	3691	3696	rVB3	896	627	0.03%	0.004%
88	12.985	3712	3715	3716	rBV2	514	283	0.01%	0.002%
89	13.024	3724	3727	3729	rVB4	803	469	0.02%	0.003%
90	13.056	3734	3737	3739	rBV3	839	657	0.03%	0.004%
91	13.741	3945	3950	3952	rBV4	1039	804	0.04%	0.005%
92	13.947	4012	4014	4016	rVB3	908	345	0.02%	0.002%
93	13.985	4024	4026	4028	rBV	636	263	0.01%	0.002%
94	14.053	4045	4047	4051	rVB3	855	426	0.02%	0.003%
95	14.120	4067	4068	4070	rBV2	664	290	0.01%	0.002%
96	14.226	4100	4101	4104	rBV3	620	304	0.01%	0.002%
97	14.464	4173	4175	4177	rBV2	694	269	0.01%	0.002%
98	14.718	4250	4254	4257	rBV3	680	705	0.03%	0.005%
99	14.995	4339	4340	4342	rBV2	668	287	0.01%	0.002%
100	15.763	4576	4579	4583	rBV5	1175	1007	0.04%	0.007%




Sum of corrected areas: 15025146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027214.D
Acq On : 04 Aug 2022 17:56
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

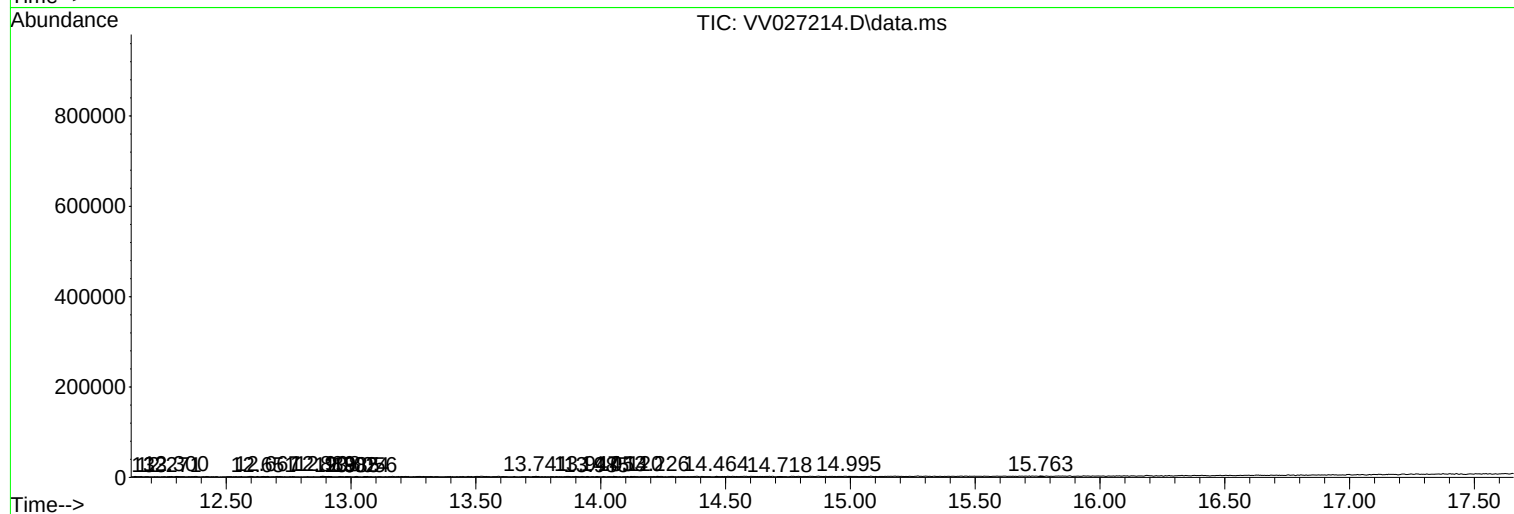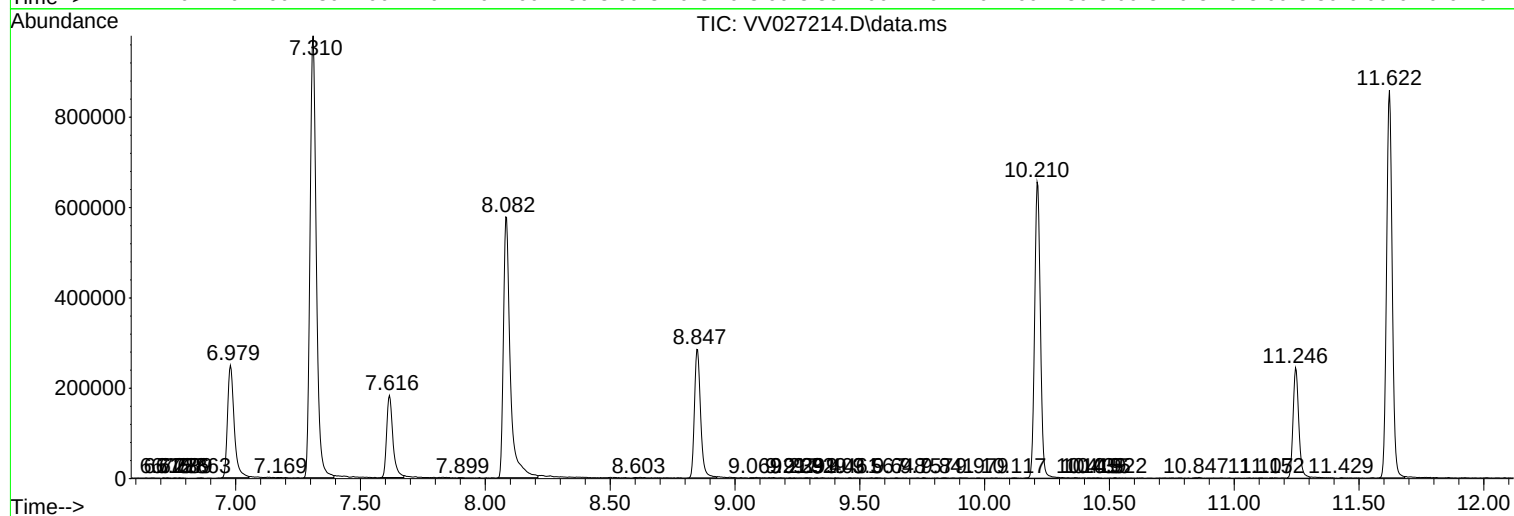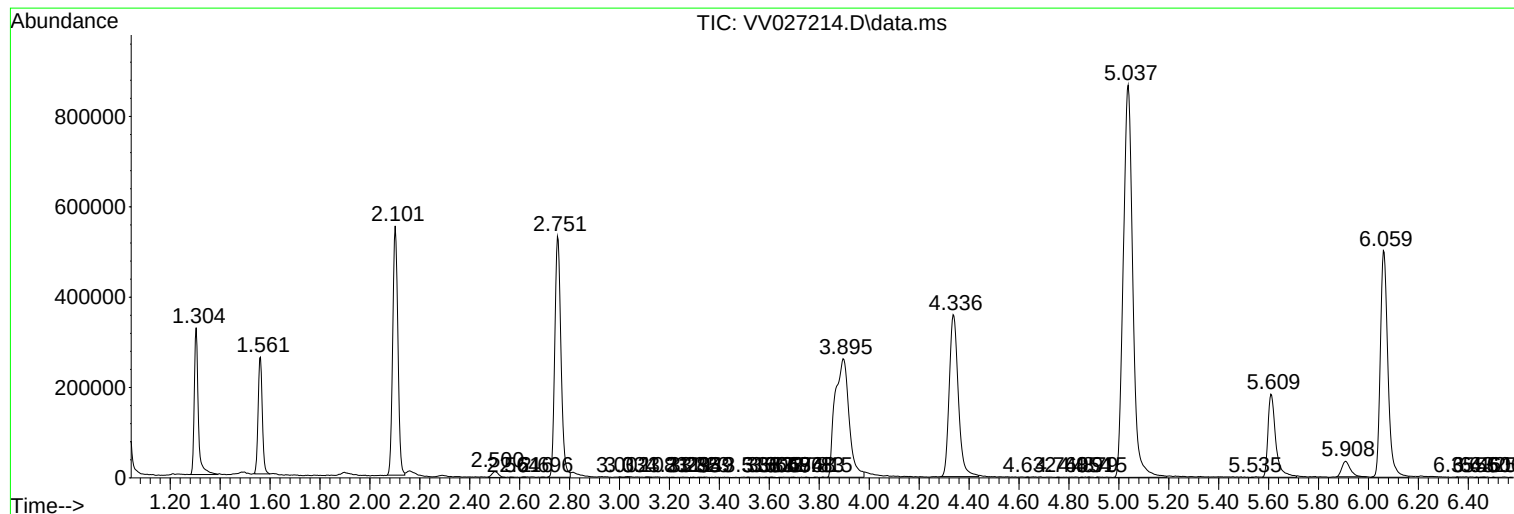

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027214.D
Acq On : 04 Aug 2022 17:56
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080422\
Data File : VV027214.D
Acq On : 04 Aug 2022 17:56
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------