

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080521\
 Data File : VV021741.D
 Acq On : 05 Aug 2021 12:31
 Operator : SY/MD
 Sample : VV0805WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 06 01:15:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 06 01:14:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	13385	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	12348	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6092	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	3467	0.505	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 100.000%			
4) 1,2-Dichloroethane-d4	5.042	65	3456	0.504	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 100.000%			
7) 1,2-Dichloropropane-d6	6.068	67	4694	0.517	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 104.000%			
8) Toluene-d8	7.317	98	12932	0.495	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 98.000%			
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2489	0.466	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 94.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.409	75	15	0.020	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080521\
Data File : VV021741.D
Acq On : 05 Aug 2021 12:31
Operator : SY/MD
Sample : VV0805WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 06 01:15:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 06 01:14:51 2021
Response via : Initial Calibration

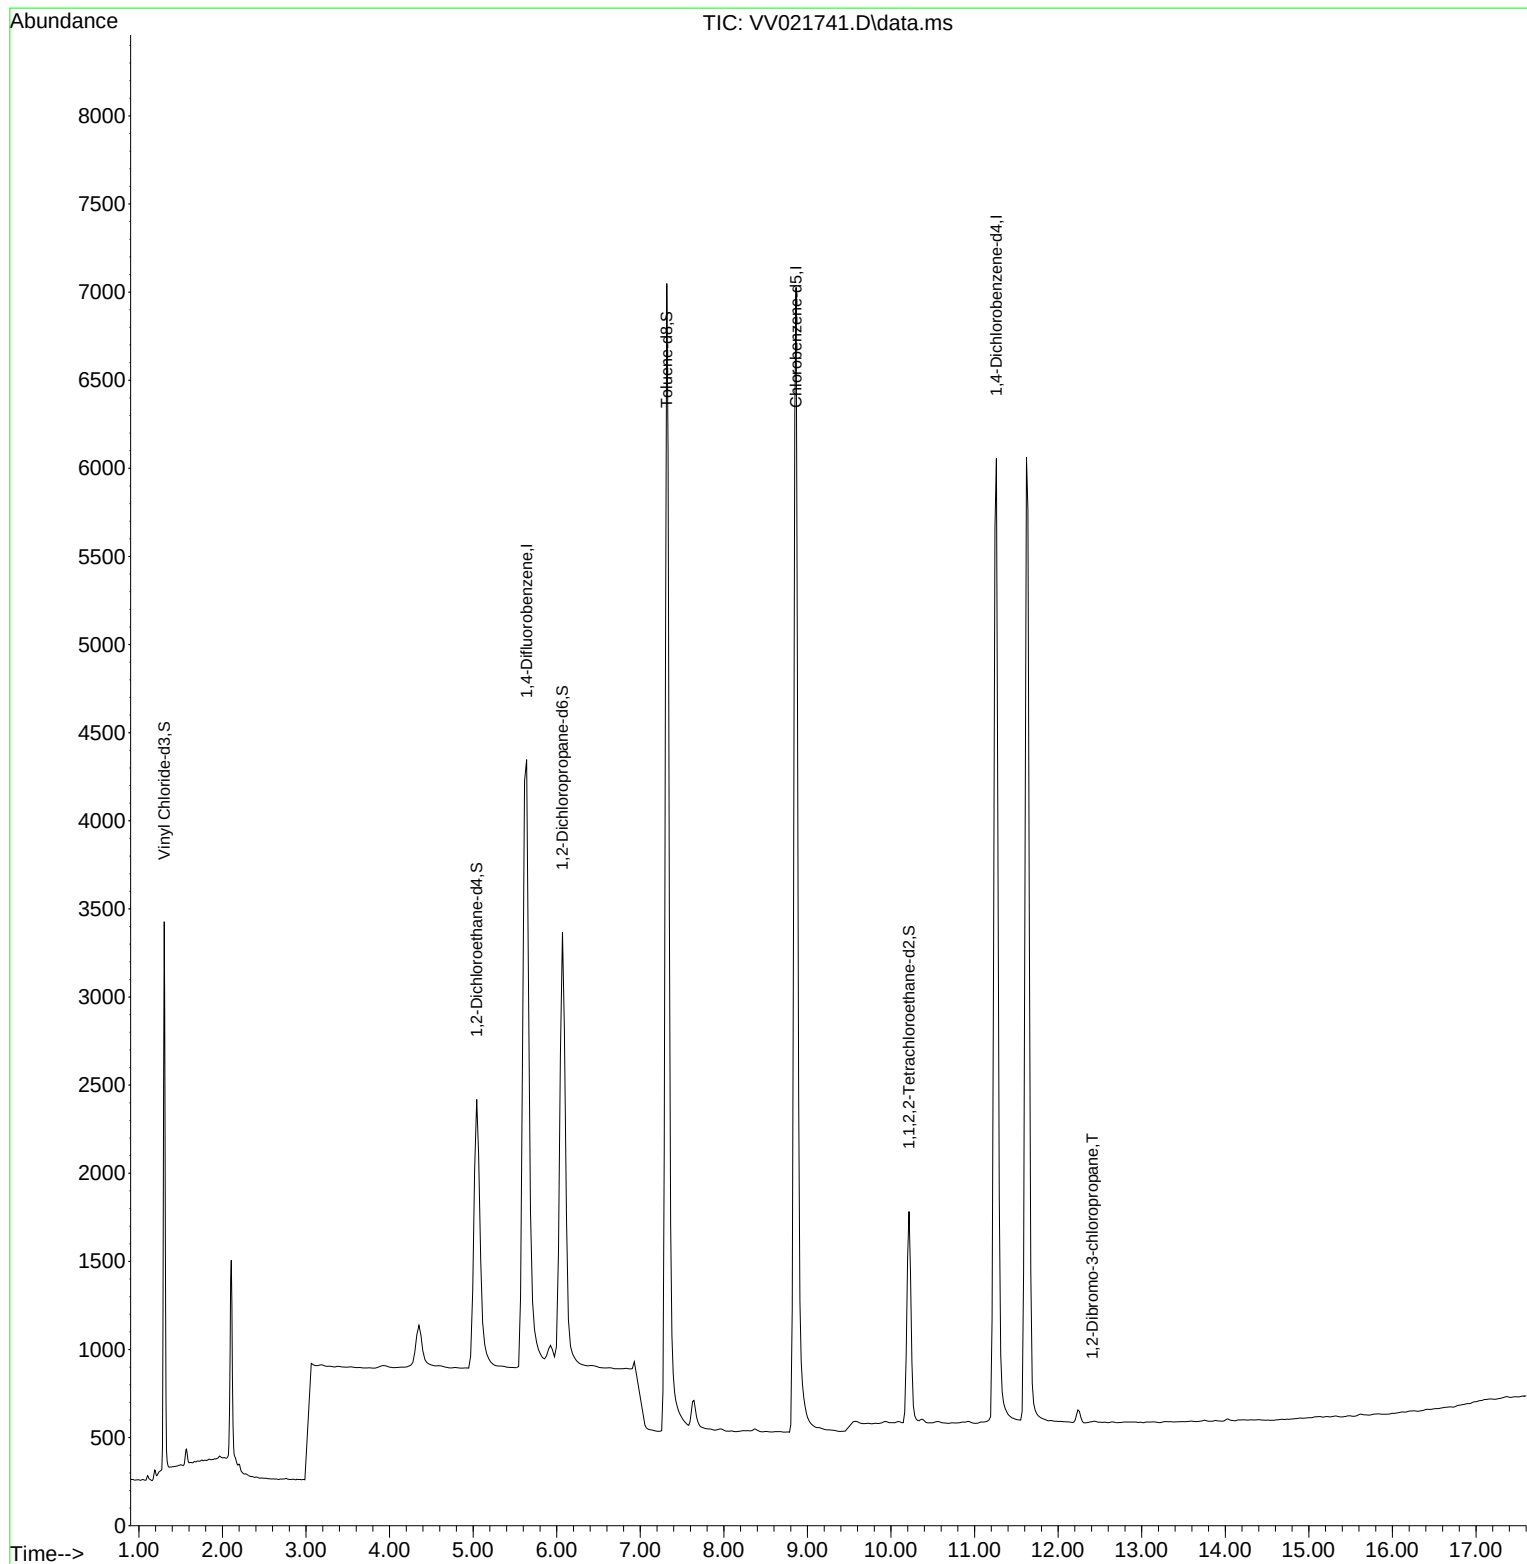

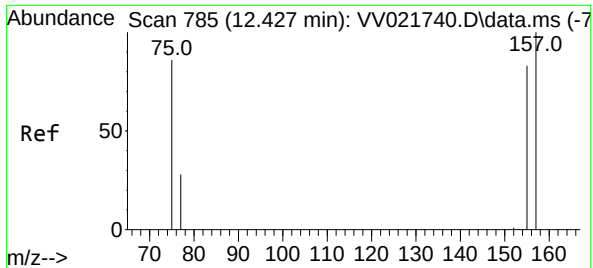

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.020 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. -0.017 min
 Lab File: VV021741.D
 Acq: 05 Aug 2021 12:31

Instrument :
 MSVOA_V
 ClientSampleId :

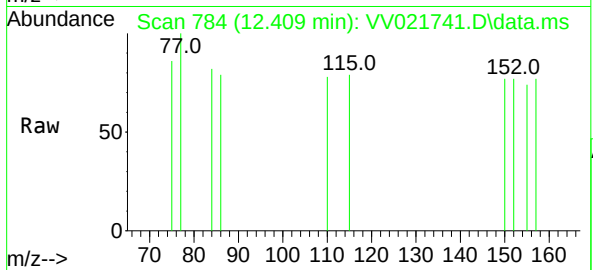

Tgt Ion:	75	Resp:	15
Ion	Ratio	Lower	Upper
75	100		
157	88.9	87.0	130.6
155	85.7	75.0	112.6

