

m/z	Abundance
40.00	133.0
44.00	542.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	732.0
37.00	3989.0
38.00	3861.0
39.00	1421.0
39.90	243.0
43.90	922.0
45.00	727.0
47.00	1230.0
47.90	531.0
49.00	3631.0
50.00	17232.0
51.00	5586.0
51.90	286.0
54.90	329.0
56.00	1393.0
57.00	2577.0
58.10	118.0
60.00	776.0
61.00	4387.0
62.00	4192.0
63.00	3572.0
63.90	407.0
65.00	410.0
67.00	197.0
68.00	9730.0
69.00	9222.0
70.00	642.0
71.90	506.0
73.00	4070.0
74.00	15494.0
75.00	47104.0
76.00	4165.0
76.90	634.0
77.90	415.0
78.90	2922.0
80.00	810.0
80.90	3140.0
81.90	706.0
86.00	111.0
86.90	4404.0
88.00	4439.0
91.00	446.0
92.00	2657.0
92.90	3945.0
94.00	11377.0
95.00	98488.0
96.00	6476.0
96.90	220.0
104.00	361.0
104.90	202.0
105.90	468.0
112.60	110.0
115.90	434.0
116.90	815.0
117.90	433.0
118.90	459.0
127.80	454.0
128.80	117.0
129.00	117.0
129.90	311.0
130.70	169.0
134.80	212.0
136.90	174.0
140.90	1111.0
141.80	151.0
142.90	1374.0
143.80	123.0
144.90	129.0
145.90	128.0
147.80	230.0
149.90	109.0
154.90	201.0
156.90	157.0
158.80	128.0
160.90	160.0
171.90	487.0
173.00	970.0
173.90	87840.0
175.00	6975.0
175.90	83456.0
177.00	5164.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	828.0
37.00	4428.0
38.00	4226.0
39.00	1491.0
39.90	239.0
44.00	1004.0
45.00	799.0
45.80	105.0
47.00	1375.0
47.90	635.0
49.00	4176.0
50.00	18896.0
51.00	6152.0
51.90	370.0
55.00	310.0
56.00	1570.0
57.00	2791.0
58.10	139.0
59.90	867.0
61.00	4689.0
62.00	4638.0
63.00	3956.0
63.90	459.0
65.00	409.0
67.10	209.0
68.00	10702.0
69.00	10204.0
70.00	725.0
72.00	456.0
73.00	4611.0
74.00	17504.0
75.00	51464.0
76.00	4586.0
77.00	666.0
77.90	500.0
78.90	3257.0
80.00	922.0
80.90	3372.0
81.90	788.0
82.70	103.0
86.00	108.0
86.90	4955.0
88.00	4928.0
90.90	463.0
92.00	3038.0
93.00	4398.0
94.00	12626.0
95.00	107560.0
96.00	7079.0
96.90	228.0
104.00	390.0
104.90	193.0
105.80	557.0
112.70	122.0
114.90	102.0
115.90	458.0
116.90	846.0
117.90	451.0
118.90	463.0
127.80	476.0
128.80	154.0
129.90	413.0
130.70	200.0
134.80	254.0
136.90	177.0
140.90	1197.0
141.70	183.0
142.90	1513.0
143.80	122.0
145.10	120.0
145.90	121.0
147.80	224.0
149.90	116.0
154.90	234.0
156.90	176.0
158.80	136.0
160.90	189.0
171.90	526.0
173.00	1009.0
173.90	94056.0
175.00	7750.0
175.90	89712.0
177.00	5318.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	791.0
37.00	4505.0
38.00	4083.0
39.00	1463.0
40.00	246.0
44.00	1005.0
45.00	812.0
45.80	124.0
47.00	1345.0
47.90	691.0
49.00	4110.0
50.00	18872.0
51.00	6211.0
51.90	388.0
55.00	272.0
56.00	1546.0
57.00	2727.0
58.10	147.0
59.90	1018.0
61.00	4610.0
62.00	4648.0
63.00	3842.0
63.90	473.0
64.90	349.0
67.10	246.0
68.00	10425.0
69.00	10359.0
70.00	727.0
72.00	438.0
73.00	4665.0
74.00	18216.0
75.00	51648.0
76.00	4556.0
77.00	639.0
77.90	478.0
78.90	3273.0
79.90	912.0
80.90	3322.0
81.90	764.0
86.00	112.0
86.90	4773.0
87.90	4864.0
90.90	483.0
92.00	3173.0
93.00	4521.0
94.00	12644.0
95.00	106720.0
96.00	7281.0
96.90	219.0
103.90	404.0
104.80	153.0
105.90	565.0
114.70	118.0
115.80	411.0
116.90	798.0
117.80	447.0
118.90	478.0
127.80	447.0
128.90	166.0
129.90	459.0
130.70	190.0
134.90	258.0
137.00	210.0
140.90	1139.0
141.80	177.0
142.90	1420.0
143.80	116.0
145.10	120.0
145.90	146.0
147.90	195.0
149.90	111.0
154.90	262.0
156.80	183.0
158.80	128.0
160.90	171.0
171.90	547.0
172.90	858.0
173.90	90656.0
175.00	7510.0
175.90	86600.0
177.00	5065.0
177.90	183.0



Instrument :
MSVOA_V
ClientSampleId :
BFB203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080521\
 Data File : VV021739.D
 Acq On : 05 Aug 2021 10:56
 Operator : SY/MD
 Sample : BFB203
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB203

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM080421.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 06 01:25:29 2021

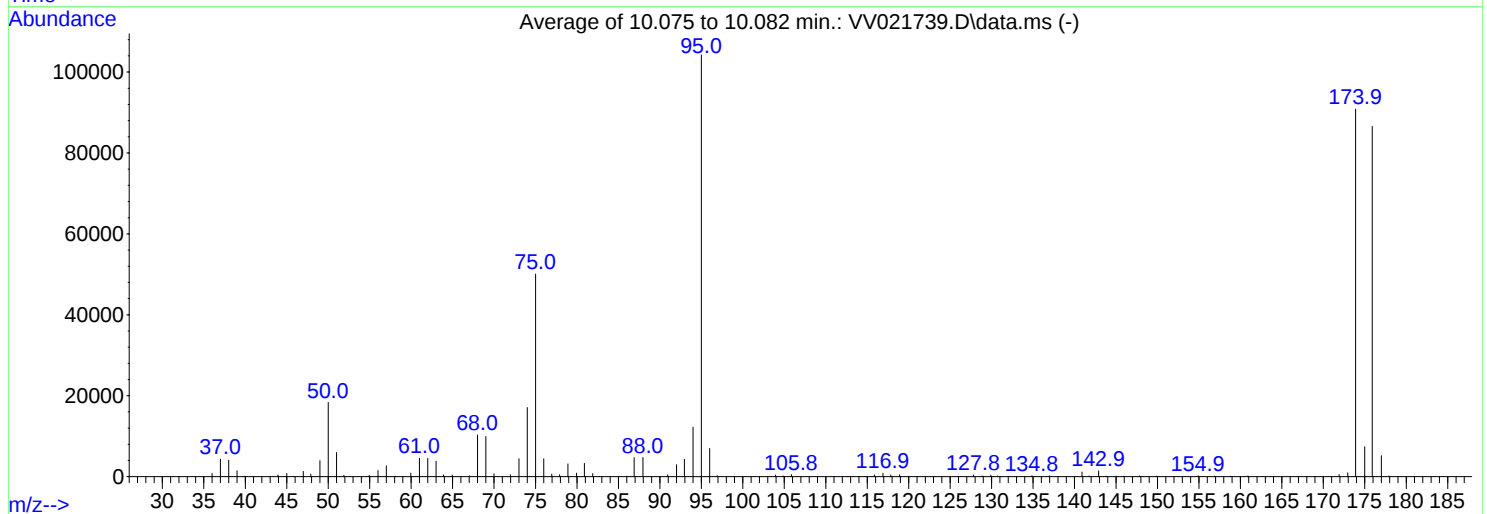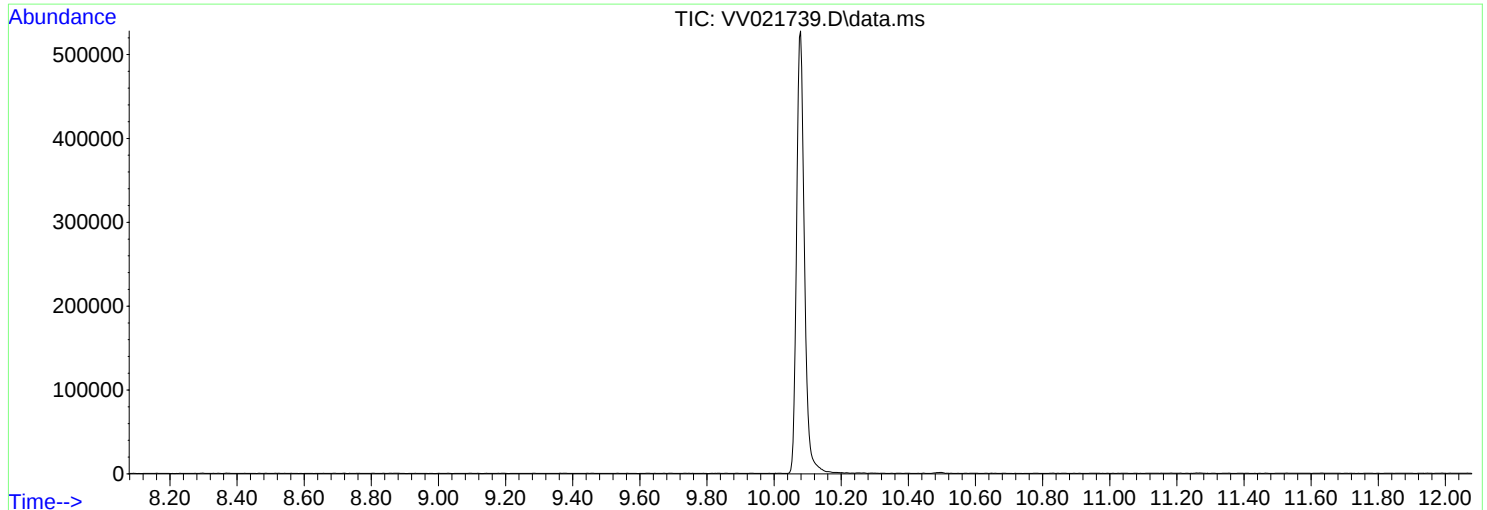

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	18333	PASS
75	95	30	80	48.0	50072	PASS
95	95	100	100	100.0	104256	PASS
96	95	5	9	6.7	6945	PASS
173	174	0.00	2	1.0	946	PASS
174	95	50	120	87.1	90851	PASS
175	174	5	9	8.2	7412	PASS
176	174	95	101	95.3	86589	PASS
177	176	5	9	6.0	5182	PASS