

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW080522\
 Data File : VW027226.D
 Acq On : 05 Aug 2022 15:42
 Operator : SY/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D47

Quant Time: Aug 06 04:00:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 06 03:57:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	320244	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	323096	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	125607	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	151967	69.602	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 139.200%#		
7) Chloroethane-d5	1.558	69	114315	71.619	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 143.240%#		
11) 1,1-Dichloroethene-d2	2.101	63	198303	49.654	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 99.300%		
21) 2-Butanone-d5	3.870	46	225876	116.224	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 116.220%		
24) Chloroform-d	4.342	84	262341	58.658	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 117.320%		
26) 1,2-Dichloroethane-d4	5.024	65	174758	62.936	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 125.880%#		
32) Benzene-d6	5.043	84	523652	67.585	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 135.160%#		
36) 1,2-Dichloropropane-d6	6.066	67	183297	66.505	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 133.020%#		
41) Toluene-d8	7.313	98	432771	65.529	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 131.060%#		
43) trans-1,3-Dichloroprop...	7.619	79	72728	60.540	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 121.080%		
47) 2-Hexanone-d5	8.088	63	133053	100.232	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 100.230%		
56) 1,1,2,2-Tetrachloroeth...	10.213	84	240517	53.550	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 107.100%		
66) 1,2-Dichlorobenzene-d4	11.622	152	150027	69.165	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 138.340%#		
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.307	62	7846	2.420	ug/L	# 76
13) Acetone	2.156	43	13890	9.269	ug/L	85
17) trans-1,2-Dichloroethene	2.757	96	13427	5.468	ug/L	83
20) cis-1,2-Dichloroethene	3.902	96	307109	120.394	ug/L	87
34) Trichloroethene	5.911	95	59942	22.547	ug/L	95
46) Tetrachloroethene	7.979	164	2305	1.185	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027226.D
Acq On : 05 Aug 2022 15:42
Operator : SY/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D47

Quant Time: Aug 06 04:00:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 06 03:57:43 2022
Response via : Initial Calibration




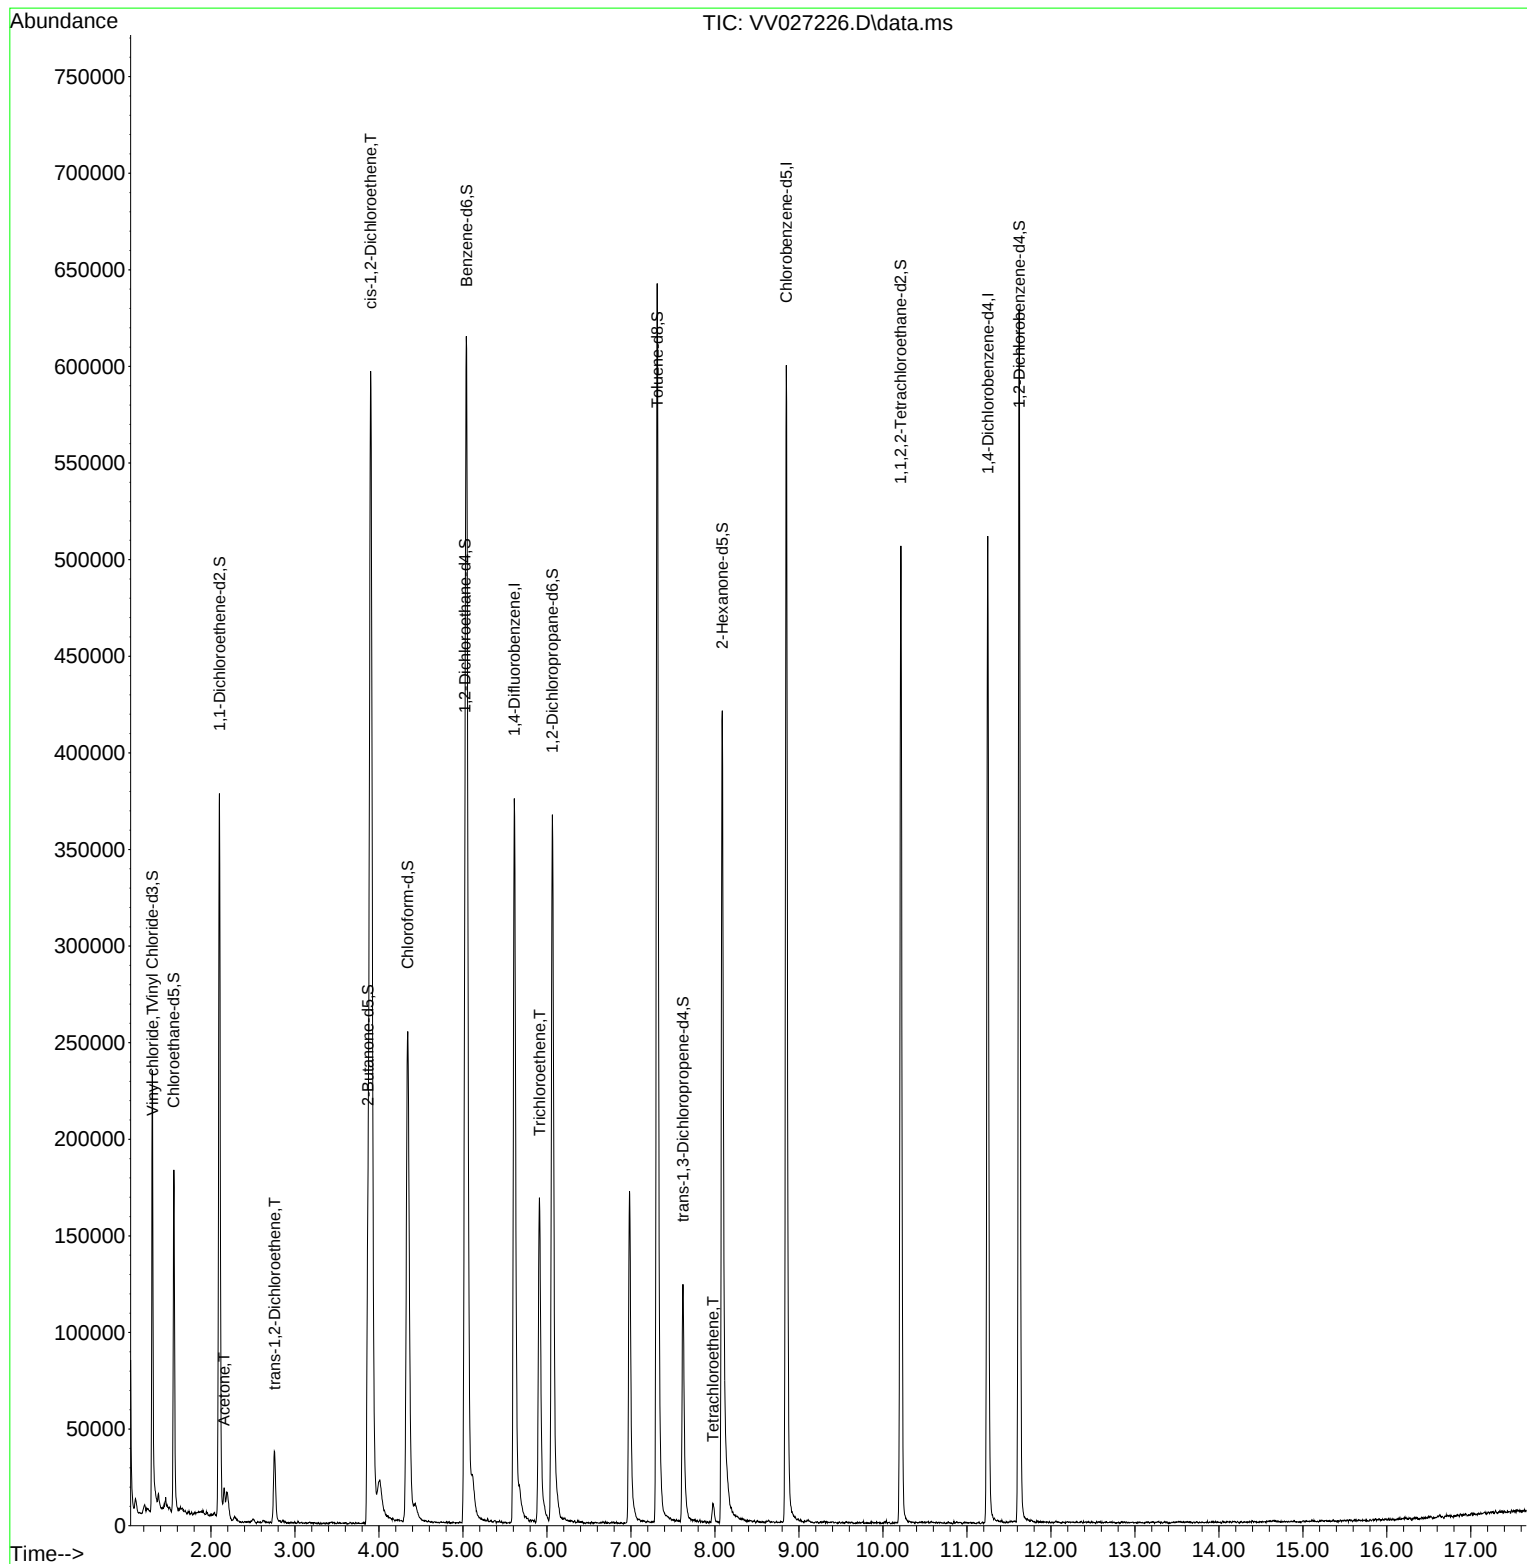


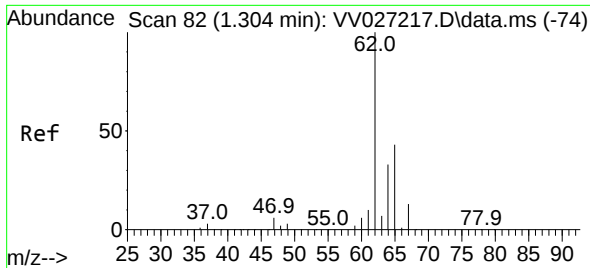

#5
 Vinyl chloride
 Concen: 2.420 ug/L
 RT: 1.307 min Scan# 81
 Delta R.T. 0.003 min
 Lab File: VV027226.D
 Acq: 05 Aug 2022 15:42




Instrument :
 MSVOA_V
 ClientSampleId :
 F5D47


Tgt Ion: 62 Resp: 7846
 Ion Ratio Lower Upper
 62 100
 64 46.7 23.2 43.2#

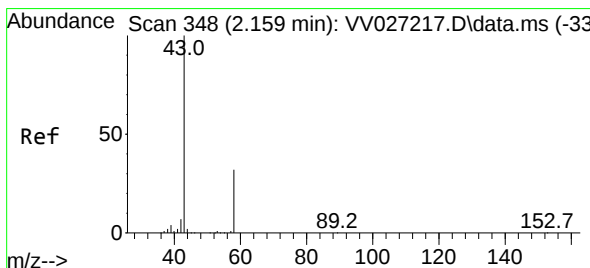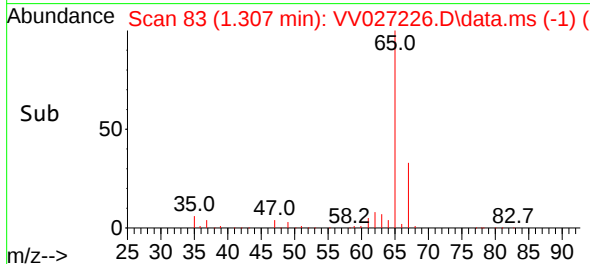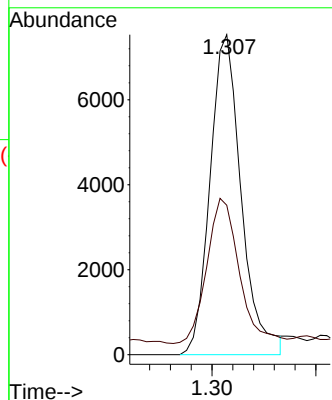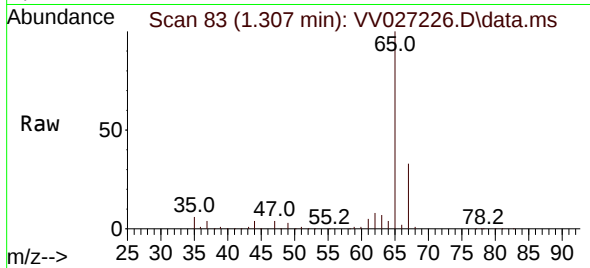

#13
 Acetone
 Concen: 9.269 ug/L
 RT: 2.156 min Scan# 347
 Delta R.T. -0.003 min
 Lab File: VV027226.D
 Acq: 05 Aug 2022 15:42

Tgt Ion: 43 Resp: 13890
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 49.6


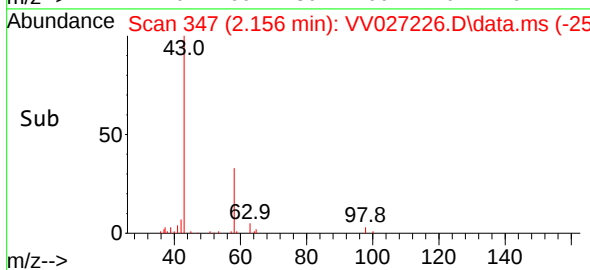
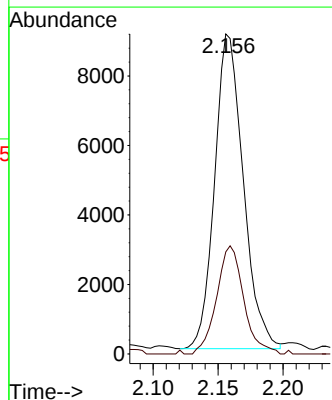
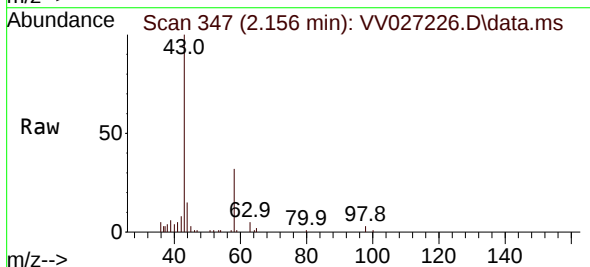


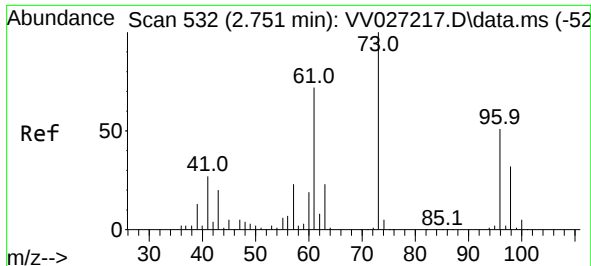

#17
trans-1,2-Dichloroethene
Concen: 5.468 ug/L
RT: 2.757 min Scan# 51
Delta R.T. 0.006 min
Lab File: VV027226.D
Acq: 05 Aug 2022 15:42




Instrument :
MSVOA_V
ClientSampleId :
F5D47


Tgt Ion: 96 Resp: 13427
Ion Ratio Lower Upper
96 100
61 150.7 89.2 165.6
98 72.8 44.6 82.8

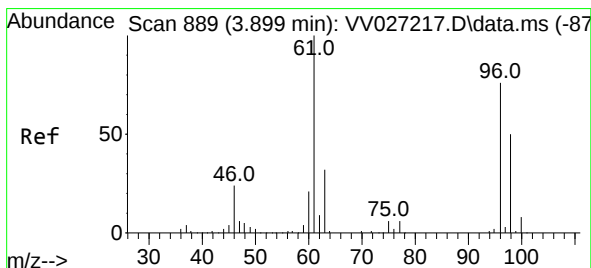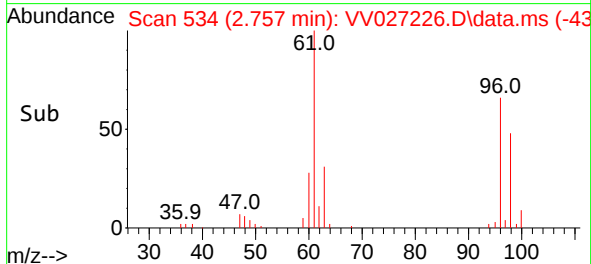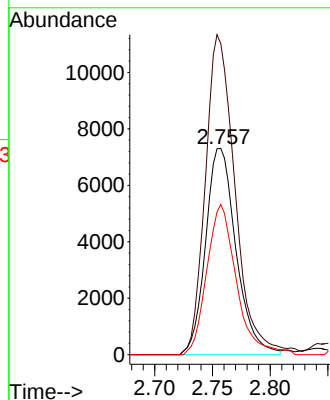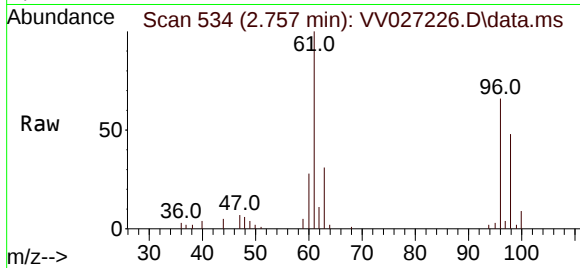

#20
cis-1,2-Dichloroethene
Concen: 120.394 ug/L
RT: 3.902 min Scan# 890
Delta R.T. 0.003 min
Lab File: VV027226.D
Acq: 05 Aug 2022 15:42

Tgt Ion: 96 Resp: 307109
Ion Ratio Lower Upper
96 100
61 131.2 81.8 151.8
68 0.0 0.0 0.0

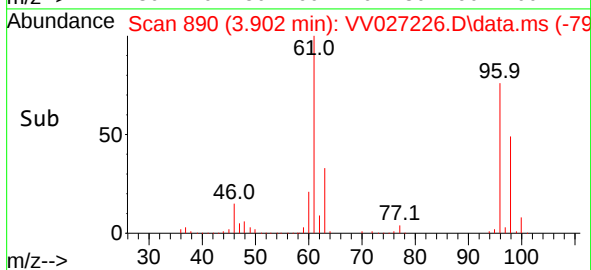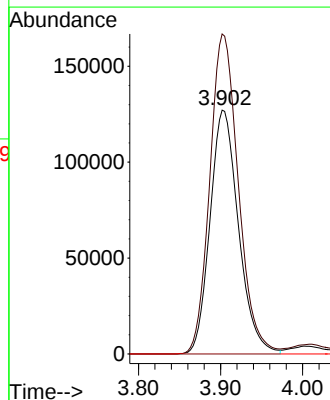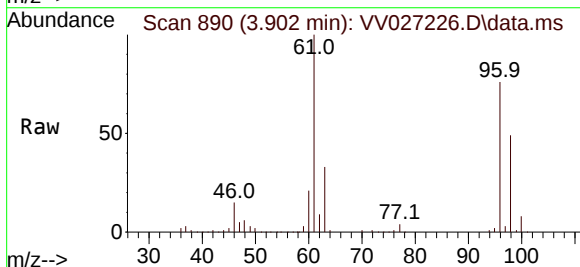

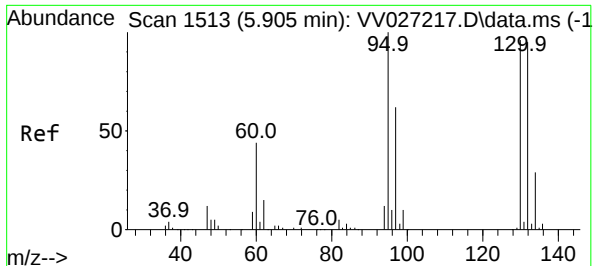

#34

Trichloroethene

Concen: 22.547 ug/L

RT: 5.911 min Scan# 1

Delta R.T. 0.006 min

Lab File: VV027226.D

Acq: 05 Aug 2022 15:42

Instrument :

MSVOA_V

ClientSampleId :

F5D47

Tgt Ion: 95 Resp: 59942





Ion Ratio Lower Upper

95 100

97 63.9 45.9 85.3

132 93.0 69.8 129.6

130 97.6 72.5 134.7

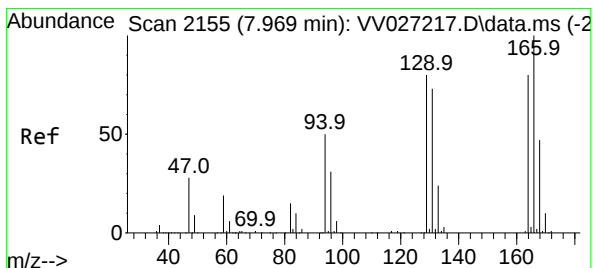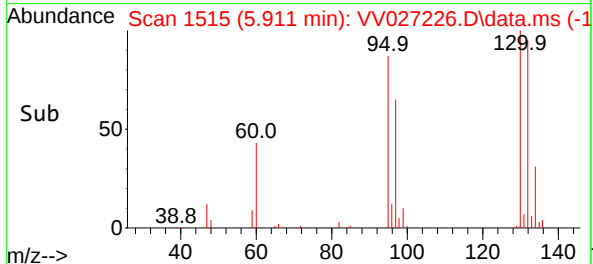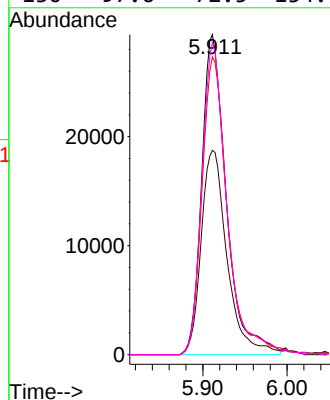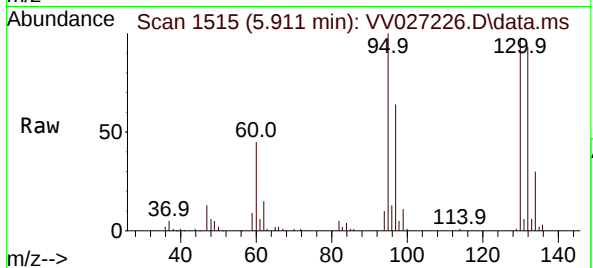

#46

Tetrachloroethene

Concen: 1.185 ug/L

RT: 7.979 min Scan# 2158

Delta R.T. 0.010 min

Lab File: VV027226.D

Acq: 05 Aug 2022 15:42

Tgt Ion:164 Resp: 2305

Ion Ratio Lower Upper

164 100

129 84.0 67.5 125.4

131 70.2 64.3 119.3

166 102.7 88.9 165.1

