

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027220.D
 Acq On : 05 Aug 2022 12:24
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV2	524014	592894	42.86%	5.293%
2	1.558	155	161	178	rVB	143649	169366	12.24%	1.512%
3	2.098	320	329	344	rBV	261013	366835	26.52%	3.275%
4	2.500	444	454	466	rBV2	12492	20921	1.51%	0.187%
5	2.754	525	533	549	rVB	23866	42981	3.11%	0.384%
6	2.876	569	571	576	rVB5	781	613	0.04%	0.005%
7	2.912	580	582	585	rBV4	622	356	0.03%	0.003%
8	2.957	594	596	598	rBV2	530	243	0.02%	0.002%
9	2.969	598	600	602	rVB2	791	312	0.02%	0.003%
10	3.098	638	640	643	rBV2	433	232	0.02%	0.002%
11	3.114	643	645	648	rBV2	394	325	0.02%	0.003%
12	3.188	666	668	669	rBV2	471	97	0.01%	0.001%
13	3.214	674	676	679	rVB	531	228	0.02%	0.002%
14	3.227	679	680	681	rBV	362	97	0.01%	0.001%
15	3.310	704	706	708	rVB3	523	168	0.01%	0.001%
16	3.391	730	731	734	rBV2	492	278	0.02%	0.002%
17	3.404	734	735	736	rVV	654	156	0.01%	0.001%
18	3.429	740	743	745	rVB3	526	328	0.02%	0.003%
19	3.442	745	747	750	rBV3	852	453	0.03%	0.004%
20	3.548	777	780	781	rBV2	745	395	0.03%	0.004%
21	3.567	784	786	790	rVB4	530	372	0.03%	0.003%
22	3.638	805	808	810	rBV2	542	364	0.03%	0.003%
23	3.667	816	817	819	rBV2	647	262	0.02%	0.002%
24	3.683	819	822	826	rVV3	805	738	0.05%	0.007%
25	3.770	847	849	853	rVB3	298	148	0.01%	0.001%
26	3.821	861	865	868	rBV3	507	478	0.03%	0.004%
27	3.870	870	880	914	rBV	150970	446260	32.26%	3.984%
28	4.336	1009	1025	1046	rBV	242571	610263	44.12%	5.448%
29	4.670	1126	1129	1131	rBV3	819	504	0.04%	0.004%
30	4.786	1164	1165	1167	rBV2	579	317	0.02%	0.003%
31	4.828	1176	1178	1182	rBV3	656	501	0.04%	0.004%
32	4.866	1186	1190	1195	rBV3	1019	1126	0.08%	0.010%
33	4.889	1195	1197	1200	rBV3	834	447	0.03%	0.004%
34	4.953	1215	1217	1219	rBV2	573	238	0.02%	0.002%
35	4.966	1219	1221	1224	rVV3	448	223	0.02%	0.002%
36	5.037	1226	1243	1289	rVV2	504384	1383235	100.00%	12.349%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027220.D
 Acq On : 05 Aug 2022 12:24
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	5.510	1388	1390	1394	rBV3	783	383	0.03%	0.003%
38	5.567	1405	1408	1409	rBV2	511	273	0.02%	0.002%
39	5.609	1409	1421	1453	rBV	389804	830307	60.03%	7.413%
40	5.902	1503	1512	1521	rBV3	11772	24066	1.74%	0.215%
41	6.063	1549	1562	1590	rBV	337350	704288	50.92%	6.288%
42	6.587	1721	1725	1731	rBV6	773	864	0.06%	0.008%
43	6.651	1742	1745	1746	rBV2	625	347	0.03%	0.003%
44	6.706	1758	1762	1765	rBV4	674	537	0.04%	0.005%
45	6.741	1772	1773	1776	rBV2	439	264	0.02%	0.002%
46	6.757	1776	1778	1780	rBV	808	417	0.03%	0.004%
47	6.908	1820	1825	1827	rBV3	1081	883	0.06%	0.008%
48	6.982	1837	1848	1872	rBV	149196	288835	20.88%	2.579%
49	7.230	1923	1925	1927	rBV2	545	238	0.02%	0.002%
50	7.310	1939	1950	1977	rBV	477951	859007	62.10%	7.669%
51	7.616	2036	2045	2064	rBV	112589	206688	14.94%	1.845%
52	7.960	2150	2152	2155	rBV	494	308	0.02%	0.003%
53	7.998	2161	2164	2166	rVB3	683	351	0.03%	0.003%
54	8.027	2171	2173	2174	rBV	508	198	0.01%	0.002%
55	8.085	2181	2191	2224	rBV	467622	920165	66.52%	8.215%
56	8.677	2373	2375	2376	rBV	635	300	0.02%	0.003%
57	8.850	2417	2429	2452	rBV	608804	1026756	74.23%	9.167%
58	9.361	2585	2588	2591	rBV3	522	347	0.03%	0.003%
59	9.480	2623	2625	2628	rBV3	508	286	0.02%	0.003%
60	9.516	2632	2636	2638	rBV3	759	546	0.04%	0.005%
61	9.699	2691	2693	2695	rBV	683	258	0.02%	0.002%
62	9.725	2699	2701	2703	rBV2	317	123	0.01%	0.001%
63	9.747	2705	2708	2712	rVB2	731	483	0.03%	0.004%
64	9.786	2718	2720	2722	rBV2	625	249	0.02%	0.002%
65	9.834	2733	2735	2736	rVB	602	148	0.01%	0.001%
66	9.892	2750	2753	2755	rBV5	745	471	0.03%	0.004%
67	10.162	2835	2837	2840	rBV4	407	276	0.02%	0.002%
68	10.214	2840	2853	2875	rVV	548232	867747	62.73%	7.747%
69	10.429	2918	2920	2921	rVB2	476	102	0.01%	0.001%
70	10.442	2922	2924	2925	rVV	725	210	0.02%	0.002%
71	10.519	2947	2948	2951	rVB	507	202	0.01%	0.002%
72	10.538	2951	2954	2955	rBV2	681	400	0.03%	0.004%
73	10.805	3034	3037	3038	rBV	946	490	0.04%	0.004%
74	10.959	3083	3085	3086	rBV2	567	163	0.01%	0.001%
75	11.107	3127	3131	3133	rBV3	839	512	0.04%	0.005%
76	11.204	3159	3161	3163	rBV	662	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027220.D
 Acq On : 05 Aug 2022 12:24
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3194	rBV	545963	830149	60.02%	7.411%
78	11.529	3261	3262	3264	rBV	560	206	0.01%	0.002%
79	11.622	3278	3291	3310	rBV	616631	986491	71.32%	8.807%
80	12.172	3461	3462	3463	rBV	515	187	0.01%	0.002%
81	12.342	3511	3515	3518	rBV2	776	487	0.04%	0.004%
82	12.905	3689	3690	3692	rBV2	664	294	0.02%	0.003%
83	13.709	3938	3940	3941	rBV	583	193	0.01%	0.002%
84	13.754	3952	3954	3958	rBV3	846	617	0.04%	0.006%
85	14.117	4064	4067	4068	rBV2	977	445	0.03%	0.004%
86	14.358	4140	4142	4144	rBV2	783	354	0.03%	0.003%


Sum of corrected areas: 11200921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027220.D
Acq On : 05 Aug 2022 12:24
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

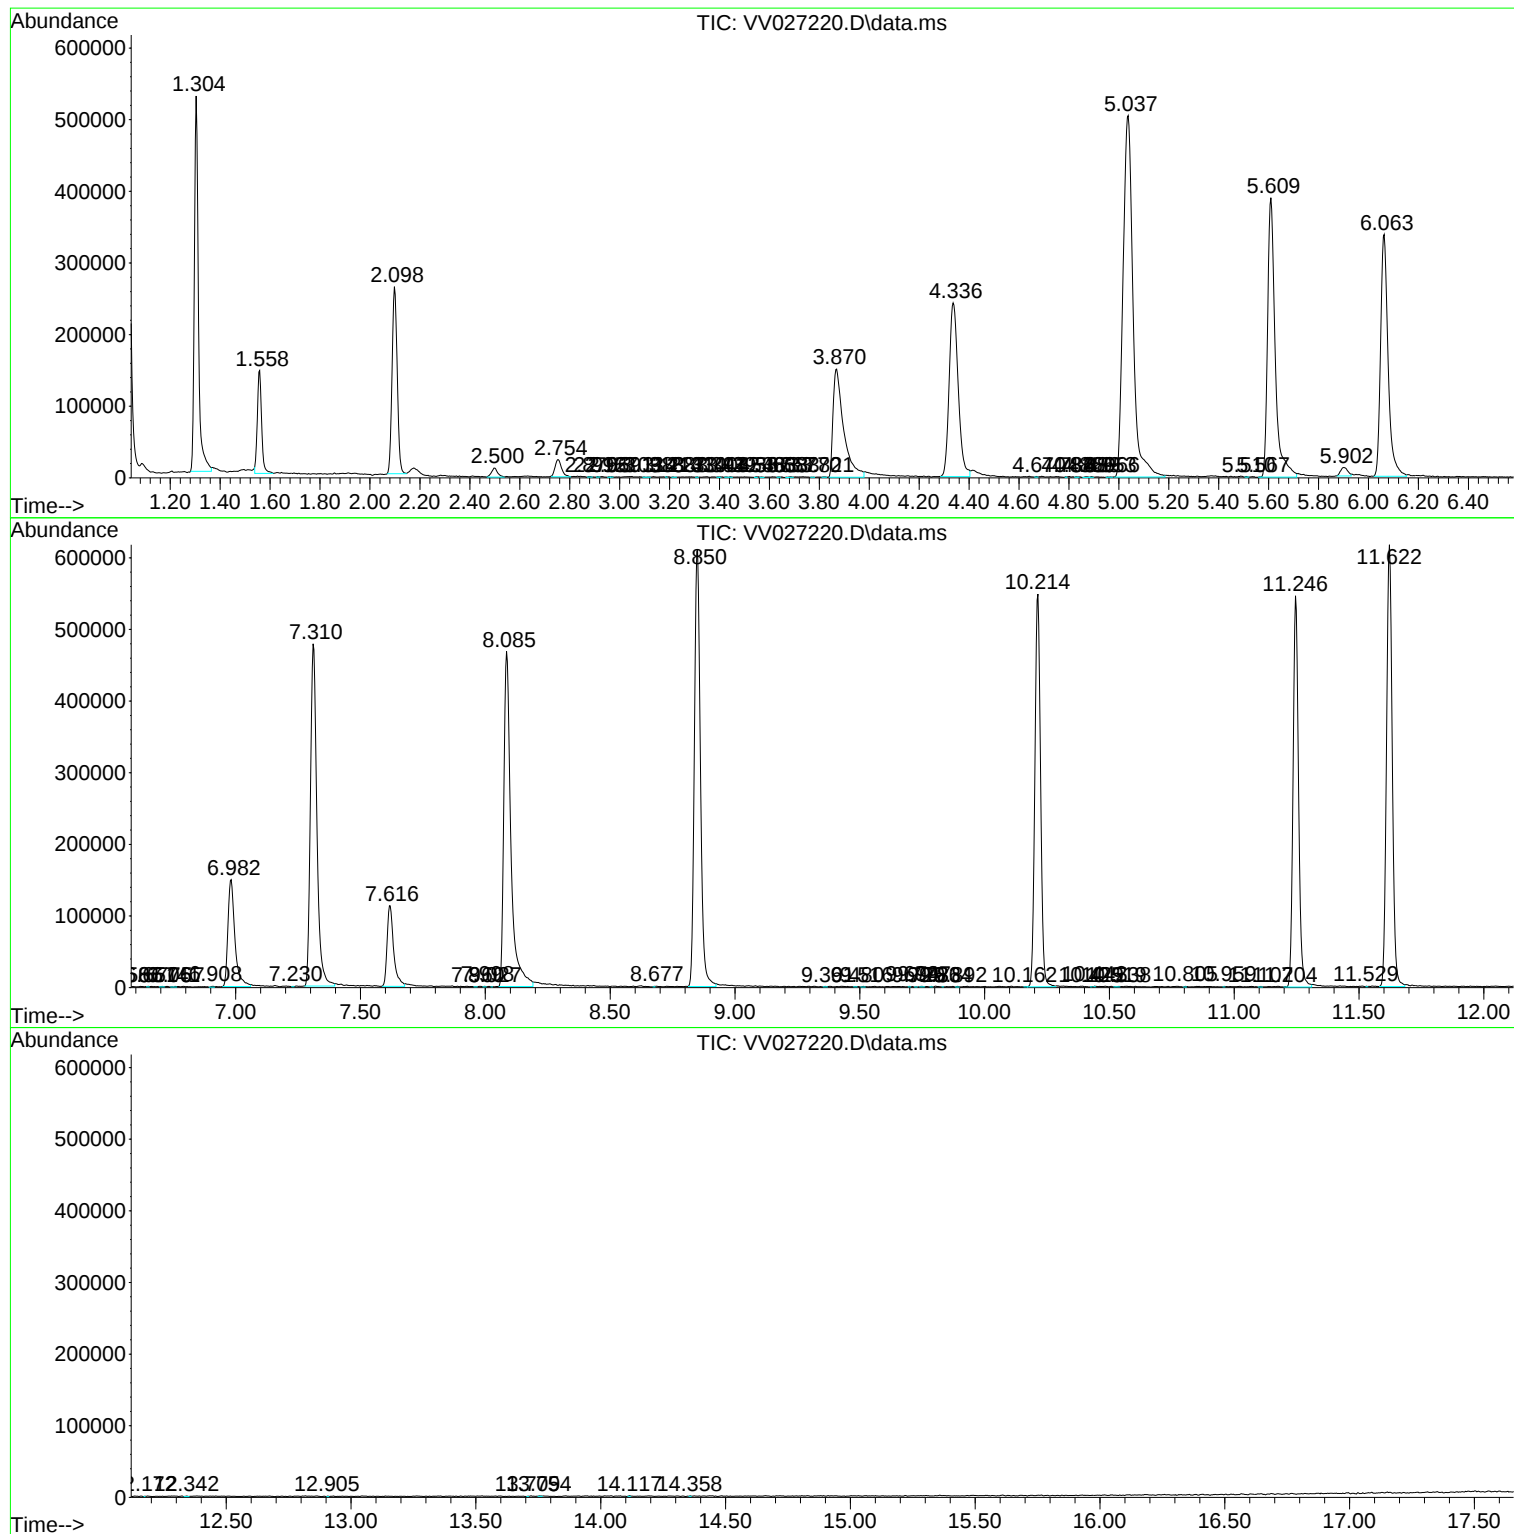

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027220.D
Acq On : 05 Aug 2022 12:24
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027220.D
Acq On : 05 Aug 2022 12:24
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc