

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027221.D
 Acq On : 05 Aug 2022 12:48
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	121286	134990	12.22%	1.264%
2	1.561	156	162	173	rVB	111567	126317	11.43%	1.182%
3	2.101	321	330	347	rVB	200418	286254	25.91%	2.679%
4	2.503	449	455	470	rVB2	10982	18981	1.72%	0.178%
5	2.561	470	473	479	rBV5	1200	1050	0.10%	0.010%
6	2.616	481	490	491	rBV9	1423	1672	0.15%	0.016%
7	2.696	512	515	518	rBV3	524	405	0.04%	0.004%
8	2.754	518	533	553	rBV	623292	1077625	97.53%	10.087%
9	3.008	609	612	614	rBV3	944	506	0.05%	0.005%
10	3.079	632	634	638	rVB3	1040	635	0.06%	0.006%
11	3.330	709	712	713	rBV2	485	269	0.02%	0.003%
12	3.368	721	724	728	rBV4	850	479	0.04%	0.004%
13	3.526	770	773	775	rBV3	735	515	0.05%	0.005%
14	3.561	783	784	788	rBV2	459	323	0.03%	0.003%
15	3.741	837	840	843	rBV2	564	332	0.03%	0.003%
16	3.831	865	868	870	rBV3	652	314	0.03%	0.003%
17	3.902	871	890	915	rBV3	265207	894719	80.98%	8.375%
18	4.275	1004	1006	1008	rBV3	1063	491	0.04%	0.005%
19	4.343	1013	1027	1049	rVV	190369	465587	42.14%	4.358%
20	4.606	1107	1109	1112	rBV4	567	299	0.03%	0.003%
21	4.629	1114	1116	1121	rBV4	586	515	0.05%	0.005%
22	4.786	1163	1165	1171	rVB5	847	583	0.05%	0.005%
23	4.815	1171	1174	1175	rBV2	626	364	0.03%	0.003%
24	4.889	1194	1197	1198	rBV3	514	342	0.03%	0.003%
25	4.973	1220	1223	1225	rBV2	493	266	0.02%	0.002%
26	5.040	1228	1244	1263	rBV2	390681	1027880	93.03%	9.621%
27	5.471	1375	1378	1381	rVB4	694	503	0.05%	0.005%
28	5.497	1381	1386	1388	rBV4	921	744	0.07%	0.007%
29	5.555	1401	1404	1407	rVB4	716	576	0.05%	0.005%
30	5.613	1410	1422	1438	rBV	415183	842131	76.22%	7.882%
31	6.066	1549	1563	1594	rBV	258975	553410	50.09%	5.180%
32	6.272	1624	1627	1629	rBV2	1152	870	0.08%	0.008%
33	6.297	1633	1635	1637	rBV3	583	346	0.03%	0.003%
34	6.330	1643	1645	1646	rBV2	773	339	0.03%	0.003%
35	6.368	1655	1657	1658	rBV	880	364	0.03%	0.003%
36	6.461	1683	1686	1688	rBV2	877	466	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027221.D
 Acq On : 05 Aug 2022 12:48
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.545	1710	1712	1715	rBV3	536	268	0.02%	0.003%
38	6.584	1722	1724	1726	rBV3	498	272	0.02%	0.003%
39	6.683	1753	1755	1761	rVB4	795	861	0.08%	0.008%
40	6.776	1782	1784	1789	rVV5	955	703	0.06%	0.007%
41	6.796	1789	1790	1792	rVB	848	285	0.03%	0.003%
42	6.876	1812	1815	1818	rBV2	783	476	0.04%	0.004%
43	6.918	1825	1828	1830	rBV3	626	505	0.05%	0.005%
44	6.985	1836	1849	1880	rBV2	116093	231165	20.92%	2.164%
45	7.211	1915	1919	1920	rBV2	962	679	0.06%	0.006%
46	7.313	1940	1951	1977	rVV	350063	647890	58.64%	6.064%
47	7.522	2015	2016	2019	rVB3	970	427	0.04%	0.004%
48	7.571	2029	2031	2032	rBV2	593	306	0.03%	0.003%
49	7.622	2037	2047	2070	rVV	84313	158091	14.31%	1.480%
50	7.860	2118	2121	2124	rBV4	935	746	0.07%	0.007%
51	7.953	2148	2150	2154	rVB3	696	314	0.03%	0.003%
52	7.976	2154	2157	2158	rBV	614	364	0.03%	0.003%
53	8.014	2164	2169	2171	rBV4	617	529	0.05%	0.005%
54	8.088	2181	2192	2231	rBV	367598	755060	68.34%	7.067%
55	8.555	2335	2337	2338	rBV2	1046	295	0.03%	0.003%
56	8.651	2362	2367	2369	rBV3	685	502	0.05%	0.005%
57	8.738	2392	2394	2397	rVB2	737	341	0.03%	0.003%
58	8.789	2407	2410	2413	rBV3	581	485	0.04%	0.005%
59	8.850	2417	2429	2452	rBV	670273	1104898	100.00%	10.342%
60	9.278	2558	2562	2565	rBV2	646	414	0.04%	0.004%
61	9.352	2583	2585	2589	rVB5	750	452	0.04%	0.004%
62	9.410	2601	2603	2606	rBV3	662	406	0.04%	0.004%
63	9.484	2623	2626	2628	rBV2	745	444	0.04%	0.004%
64	9.577	2654	2655	2657	rVB	902	302	0.03%	0.003%
65	9.593	2657	2660	2663	rBV5	645	462	0.04%	0.004%
66	9.619	2665	2668	2671	rBV3	624	460	0.04%	0.004%
67	9.667	2680	2683	2687	rBV3	724	591	0.05%	0.006%
68	9.744	2705	2707	2709	rBV	568	345	0.03%	0.003%
69	9.850	2736	2740	2743	rBV6	603	604	0.05%	0.006%
70	9.915	2757	2760	2762	rBV3	886	536	0.05%	0.005%
71	9.947	2768	2770	2774	rVB3	1091	604	0.05%	0.006%
72	9.976	2774	2779	2784	rBV5	913	1010	0.09%	0.009%
73	10.143	2828	2831	2834	rVB3	655	428	0.04%	0.004%
74	10.214	2837	2853	2873	rBV	439154	698799	63.25%	6.541%
75	10.339	2889	2892	2895	rBV3	827	518	0.05%	0.005%
76	10.352	2895	2896	2902	rVV3	806	647	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027221.D
 Acq On : 05 Aug 2022 12:48
 Operator : SY/MD
 Sample : N4005-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY143DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.445	2923	2925	2927	rBV4	794	345	0.03%	0.003%
78	10.458	2927	2929	2931	rVV2	672	343	0.03%	0.003%
79	10.513	2939	2946	2947	rBV3	590	590	0.05%	0.006%
80	10.725	3010	3012	3015	rBV2	736	399	0.04%	0.004%
81	10.760	3021	3023	3028	rVB4	833	558	0.05%	0.005%
82	10.808	3035	3038	3040	rBV3	617	297	0.03%	0.003%
83	10.850	3047	3051	3053	rBV3	1034	613	0.06%	0.006%
84	10.966	3083	3087	3093	rVB4	630	645	0.06%	0.006%
85	10.998	3093	3097	3098	rBV2	781	483	0.04%	0.005%
86	11.101	3127	3129	3131	rBV2	582	287	0.03%	0.003%
87	11.140	3138	3141	3144	rBV3	627	394	0.04%	0.004%
88	11.175	3150	3152	3155	rBV4	493	302	0.03%	0.003%
89	11.246	3163	3174	3198	rBV	556504	875753	79.26%	8.197%
90	11.448	3235	3237	3242	rVB5	865	561	0.05%	0.005%
91	11.622	3280	3291	3314	rBV	467480	743286	67.27%	6.957%
92	12.088	3433	3436	3440	rBV3	788	745	0.07%	0.007%
93	12.561	3581	3583	3586	rVB2	634	358	0.03%	0.003%
94	12.779	3648	3651	3653	rVB3	865	476	0.04%	0.004%
95	12.969	3704	3710	3713	rBV4	762	799	0.07%	0.007%
96	13.750	3950	3953	3959	rVB6	804	824	0.07%	0.008%
97	13.779	3959	3962	3966	rBV5	890	603	0.05%	0.006%
98	14.078	4052	4055	4056	rBV3	608	358	0.03%	0.003%
99	14.339	4134	4136	4140	rVB3	903	388	0.04%	0.004%
100	15.136	4382	4384	4386	rBV2	860	413	0.04%	0.004%




Sum of corrected areas: 10683766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027221.D
Acq On : 05 Aug 2022 12:48
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

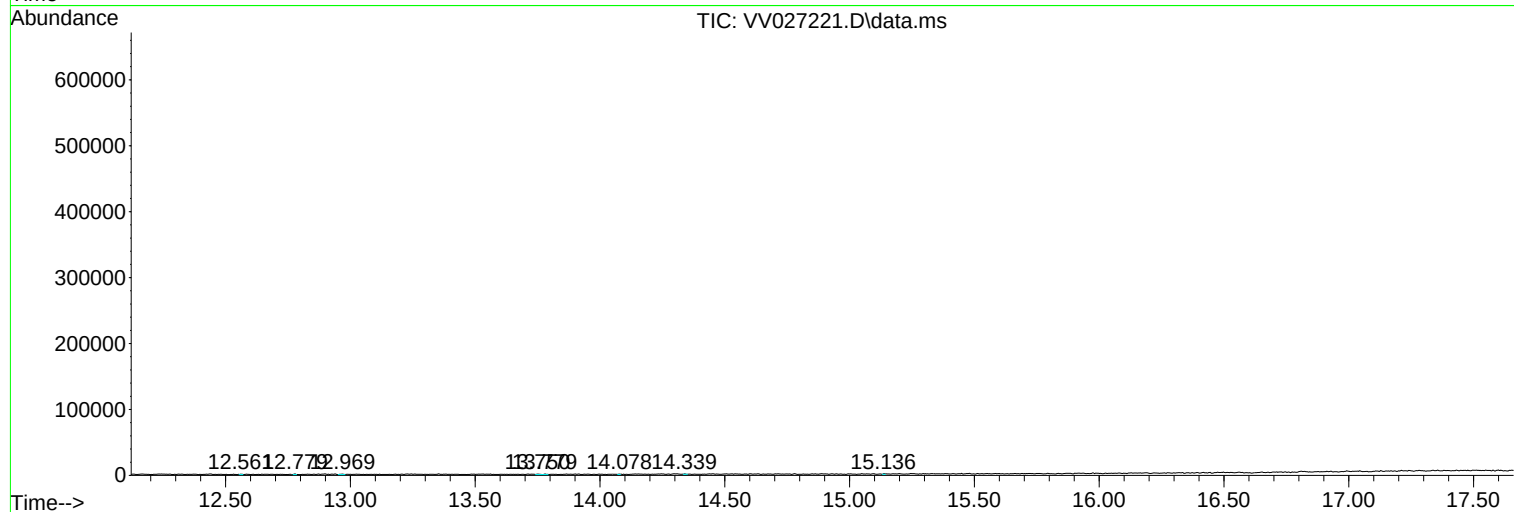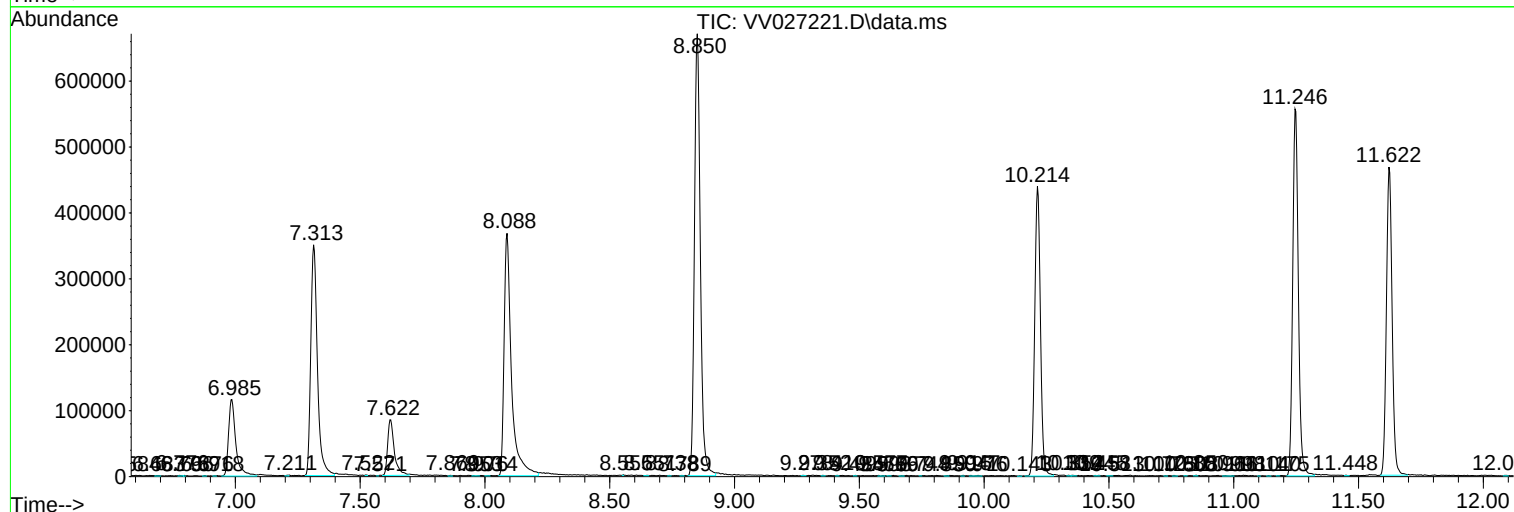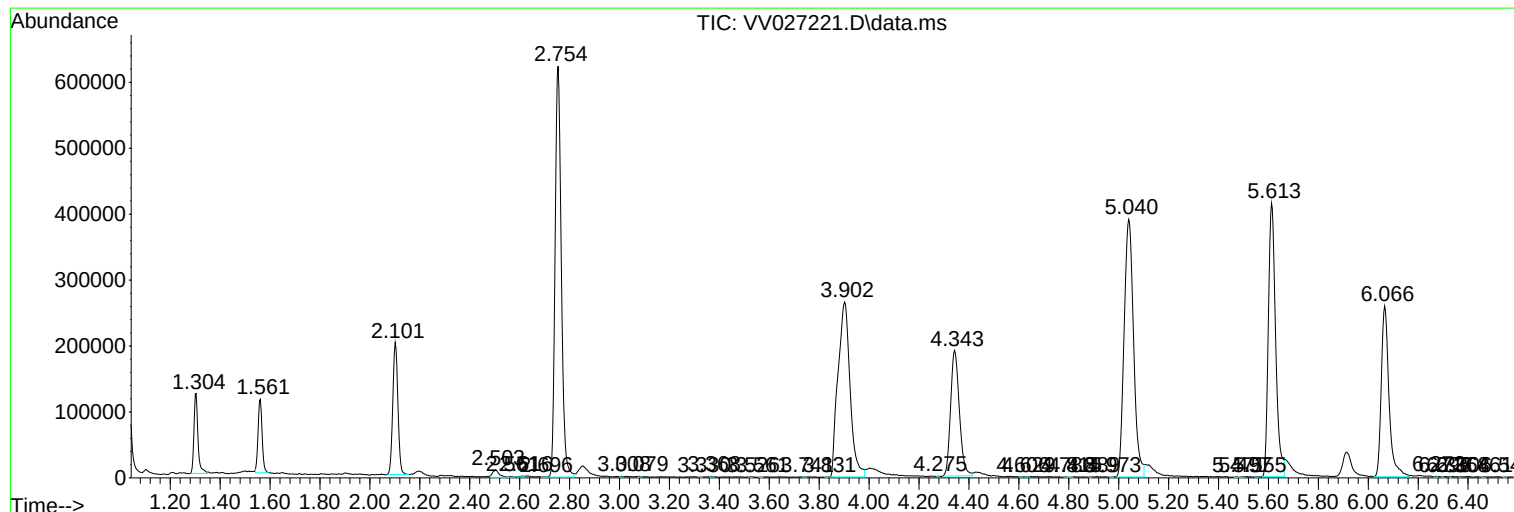

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027221.D
Acq On : 05 Aug 2022 12:48
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027221.D
Acq On : 05 Aug 2022 12:48
Operator : SY/MD
Sample : N4005-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY143DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc