

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027222.D
 Acq On : 05 Aug 2022 13:36
 Operator : SY/MD
 Sample : VIBLK271
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK271

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	100	rBV	242358	260415	15.11%	2.145%
2	1.561	155	162	172	rVB	188520	212692	12.34%	1.752%
3	2.102	320	330	345	rBV	398996	563629	32.71%	4.642%
4	2.439	432	435	442	rVB7	1130	879	0.05%	0.007%
5	2.494	445	452	453	rBV4	4191	3413	0.20%	0.028%
6	2.574	475	477	478	rBV	667	259	0.02%	0.002%
7	2.661	501	504	507	rBV3	865	600	0.03%	0.005%
8	2.909	579	581	583	rBV	524	222	0.01%	0.002%
9	3.021	610	616	617	rBV3	1190	918	0.05%	0.008%
10	3.085	635	636	637	rBV	472	113	0.01%	0.001%
11	3.095	637	639	645	rVB2	701	559	0.03%	0.005%
12	3.140	649	653	654	rBV2	604	408	0.02%	0.003%
13	3.208	672	674	676	rVB3	582	214	0.01%	0.002%
14	3.220	676	678	680	rVB	326	135	0.01%	0.001%
15	3.285	695	698	702	rBV3	952	682	0.04%	0.006%
16	3.320	706	709	713	rBV2	537	364	0.02%	0.003%
17	3.359	719	721	723	rBV2	431	268	0.02%	0.002%
18	3.372	723	725	726	rBV3	501	214	0.01%	0.002%
19	3.529	772	774	775	rBV	335	146	0.01%	0.001%
20	3.610	797	799	802	rBV2	368	206	0.01%	0.002%
21	3.655	811	813	816	rVB3	743	383	0.02%	0.003%
22	3.674	816	819	821	rBV3	386	290	0.02%	0.002%
23	3.693	823	825	832	rVB2	750	636	0.04%	0.005%
24	3.738	836	839	841	rBV2	295	188	0.01%	0.002%
25	3.754	841	844	845	rBV	385	212	0.01%	0.002%
26	3.835	864	869	870	rBV4	422	366	0.02%	0.003%
27	3.873	870	881	910	rBV2	138304	418793	24.31%	3.449%
28	4.336	1012	1025	1047	rBV	270156	665564	38.63%	5.481%
29	4.600	1106	1107	1109	rBV2	561	277	0.02%	0.002%
30	4.693	1134	1136	1138	rBV2	590	219	0.01%	0.002%
31	4.780	1161	1163	1166	rVB3	441	196	0.01%	0.002%
32	5.037	1226	1243	1290	rBV2	643209	1723001	100.00%	14.189%
33	5.455	1370	1373	1375	rBV3	1329	890	0.05%	0.007%
34	5.609	1409	1421	1455	rBV	409453	881699	51.17%	7.261%
35	5.905	1504	1513	1525	rBV4	11050	21820	1.27%	0.180%
36	6.063	1545	1562	1596	rBV	376032	812022	47.13%	6.687%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027222.D
 Acq On : 05 Aug 2022 13:36
 Operator : SY/MD
 Sample : VIBLK271
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK271

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.285	1629	1631	1637	rVB4	982	523	0.03%	0.004%
38	6.346	1646	1650	1651	rBV3	651	347	0.02%	0.003%
39	6.500	1695	1698	1699	rBV2	697	400	0.02%	0.003%
40	6.629	1729	1738	1741	rBV5	1274	1880	0.11%	0.015%
41	6.674	1748	1752	1754	rVB3	474	260	0.02%	0.002%
42	6.693	1754	1758	1759	rBV3	616	533	0.03%	0.004%
43	6.715	1763	1765	1768	rBV2	598	399	0.02%	0.003%
44	6.780	1783	1785	1786	rBV2	531	264	0.02%	0.002%
45	6.834	1800	1802	1803	rBV	511	217	0.01%	0.002%
46	6.867	1810	1812	1814	rBV3	702	252	0.01%	0.002%
47	6.889	1817	1819	1821	rBV2	496	236	0.01%	0.002%
48	6.924	1827	1830	1831	rBV3	528	218	0.01%	0.002%
49	6.979	1836	1847	1875	rBV	178174	342734	19.89%	2.822%
50	7.310	1938	1950	1982	rBV	690422	1248643	72.47%	10.283%
51	7.616	2036	2045	2074	rBV	133107	240417	13.95%	1.980%
52	8.002	2164	2165	2169	rBV3	629	251	0.01%	0.002%
53	8.085	2180	2191	2225	rBV	421338	845230	49.06%	6.961%
54	8.796	2410	2412	2413	rBV2	669	310	0.02%	0.003%
55	8.847	2417	2428	2449	rBV	674243	1108347	64.33%	9.127%
56	9.166	2525	2527	2529	rBV2	714	265	0.02%	0.002%
57	9.378	2589	2593	2596	rVB5	698	512	0.03%	0.004%
58	9.519	2633	2637	2639	rBV3	439	341	0.02%	0.003%
59	9.571	2651	2653	2657	rVB4	767	357	0.02%	0.003%
60	9.590	2657	2659	2667	rVB6	852	639	0.04%	0.005%
61	9.635	2671	2673	2674	rBV2	719	249	0.01%	0.002%
62	9.834	2733	2735	2739	rBV2	521	370	0.02%	0.003%
63	9.854	2739	2741	2742	rBV	500	187	0.01%	0.002%
64	9.957	2771	2773	2775	rVB2	1058	448	0.03%	0.004%
65	9.976	2775	2779	2781	rBV2	973	612	0.04%	0.005%
66	9.992	2781	2784	2787	rBV3	629	538	0.03%	0.004%
67	10.053	2800	2803	2804	rBV2	511	260	0.02%	0.002%
68	10.085	2810	2813	2814	rBV2	924	475	0.03%	0.004%
69	10.153	2832	2834	2835	rBV2	399	146	0.01%	0.001%
70	10.214	2841	2853	2879	rVB	504571	810436	47.04%	6.674%
71	10.429	2917	2920	2922	rBV2	674	500	0.03%	0.004%
72	10.574	2962	2965	2969	rBV4	916	691	0.04%	0.006%
73	10.654	2988	2990	2996	rVB3	1088	598	0.03%	0.005%
74	10.760	3021	3023	3029	rVB4	790	534	0.03%	0.004%
75	10.883	3059	3061	3062	rVB2	491	156	0.01%	0.001%
76	10.905	3062	3068	3073	rBV4	1015	1008	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027222.D
 Acq On : 05 Aug 2022 13:36
 Operator : SY/MD
 Sample : VIBLK271
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK271

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.928	3073	3075	3078	rBV3	789	429	0.02%	0.004%
78	10.985	3091	3093	3095	rBV	450	204	0.01%	0.002%
79	11.162	3144	3148	3149	rBV3	538	373	0.02%	0.003%
80	11.246	3163	3174	3195	rBV	572928	904486	52.49%	7.448%
81	11.529	3260	3262	3264	rBV2	801	305	0.02%	0.003%
82	11.542	3264	3266	3267	rBV	582	240	0.01%	0.002%
83	11.622	3279	3291	3307	rBV	654889	1044191	60.60%	8.599%
84	11.947	3390	3392	3396	rBV2	845	541	0.03%	0.004%
85	12.037	3418	3420	3422	rBV2	928	450	0.03%	0.004%
86	12.236	3479	3482	3488	rBV5	983	777	0.05%	0.006%
87	12.320	3506	3508	3509	rBV	562	252	0.01%	0.002%
88	12.474	3554	3556	3558	rBV	483	146	0.01%	0.001%
89	12.529	3569	3573	3576	rBV3	676	693	0.04%	0.006%
90	12.873	3678	3680	3682	rBV3	664	373	0.02%	0.003%
91	12.927	3695	3697	3698	rBV	451	192	0.01%	0.002%
92	13.448	3856	3859	3860	rBV2	490	274	0.02%	0.002%
93	13.513	3876	3879	3887	rBV3	1259	1378	0.08%	0.011%
94	13.738	3945	3949	3950	rBV3	605	379	0.02%	0.003%
95	13.789	3962	3965	3968	rBV2	989	524	0.03%	0.004%
96	13.905	3998	4001	4003	rBV3	945	622	0.04%	0.005%
97	14.001	4026	4031	4035	rVB5	1044	1095	0.06%	0.009%
98	14.062	4046	4050	4052	rBV3	676	636	0.04%	0.005%
99	14.114	4064	4066	4069	rBV2	735	412	0.02%	0.003%
100	14.394	4149	4153	4154	rBV5	931	555	0.03%	0.005%




Sum of corrected areas: 12143202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027222.D
 Acq On : 05 Aug 2022 13:36
 Operator : SY/MD
 Sample : VIBLK271
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis

TIC Library :
 TIC Integration Parameters: LSCINT.P

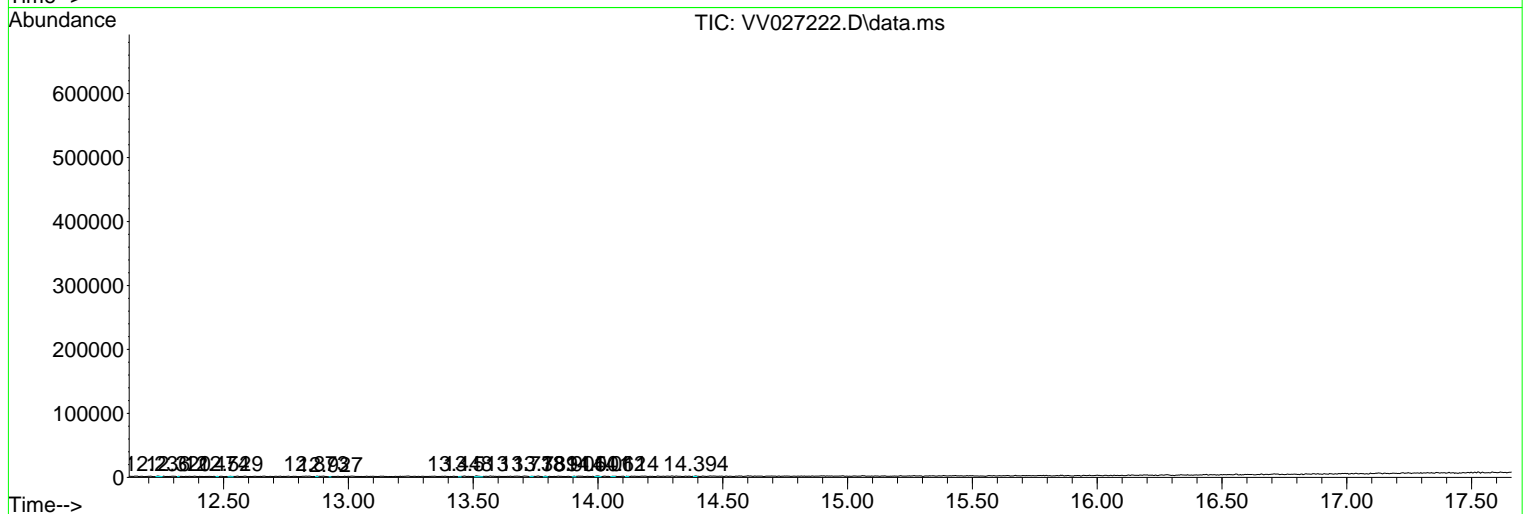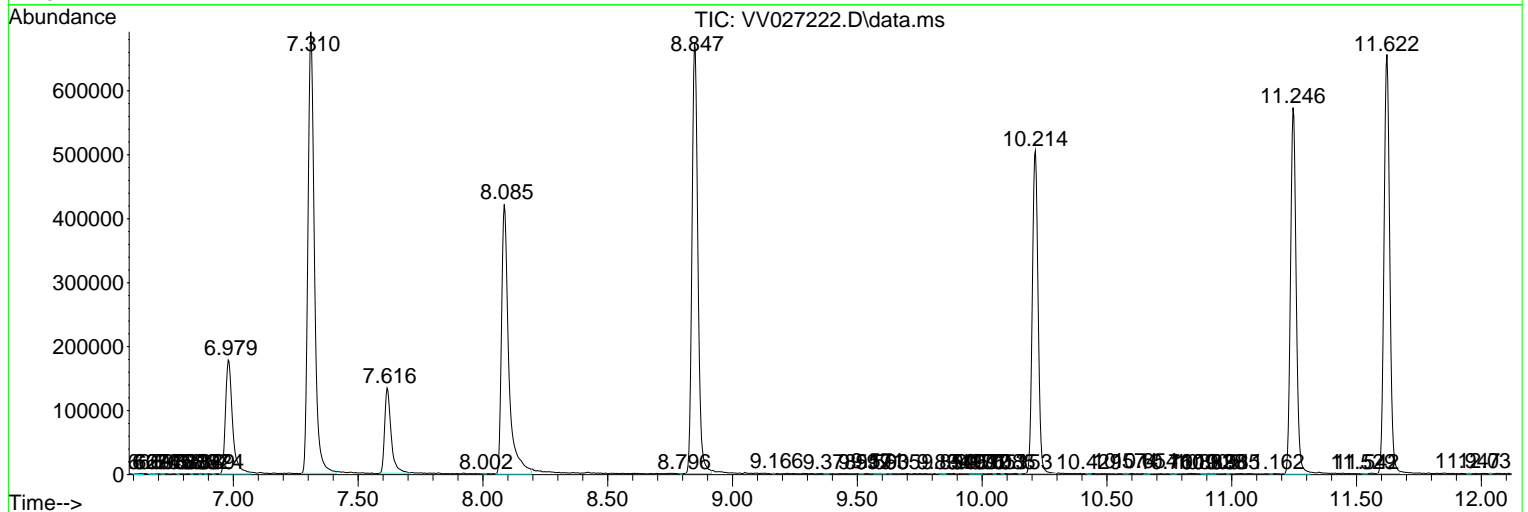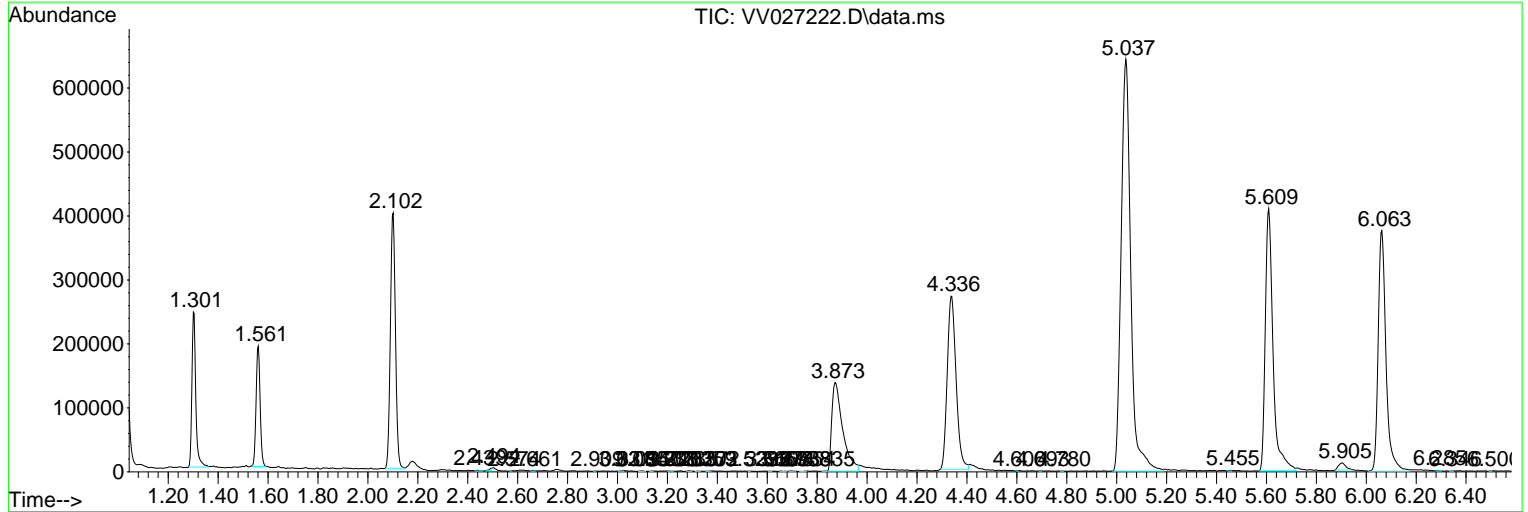

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027222.D
Acq On : 05 Aug 2022 13:36
Operator : SY/MD
Sample : VIBLK271
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027222.D
Acq On : 05 Aug 2022 13:36
Operator : SY/MD
Sample : VIBLK271
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
