

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027223.D
 Acq On : 05 Aug 2022 14:28
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rBV2	793904	908473	79.04%	8.541%
2	1.558	155	161	174	rVB	114768	132247	11.51%	1.243%
3	2.098	321	329	342	rVB	214464	305650	26.59%	2.873%
4	2.709	517	519	522	rBV3	518	308	0.03%	0.003%
5	2.754	523	533	548	rVV	26054	47050	4.09%	0.442%
6	2.931	585	588	589	rBV	673	418	0.04%	0.004%
7	3.031	616	619	622	rBV4	947	637	0.06%	0.006%
8	3.127	647	649	651	rVB2	847	305	0.03%	0.003%
9	3.413	735	738	742	rVV3	669	701	0.06%	0.007%
10	3.506	764	767	770	rBV3	596	426	0.04%	0.004%
11	3.542	775	778	781	rBV4	701	469	0.04%	0.004%
12	3.645	806	810	812	rBV2	617	311	0.03%	0.003%
13	3.661	812	815	820	rVV4	576	418	0.04%	0.004%
14	3.748	839	842	845	rBV4	1115	759	0.07%	0.007%
15	3.892	870	887	911	rBV3	163878	627892	54.63%	5.903%
16	4.336	1012	1025	1046	rBV	200583	491794	42.79%	4.623%
17	4.580	1093	1101	1103	rBV5	1143	1329	0.12%	0.012%
18	4.696	1135	1137	1139	rBV2	579	391	0.03%	0.004%
19	4.735	1144	1149	1154	rBB5	420	415	0.04%	0.004%
20	4.812	1170	1173	1175	rBV3	928	513	0.04%	0.005%
21	4.886	1192	1196	1198	rVB3	577	360	0.03%	0.003%
22	5.037	1225	1243	1283	rBV2	418905	1149369	100.00%	10.805%
23	5.497	1383	1386	1389	rBV4	970	561	0.05%	0.005%
24	5.609	1407	1421	1464	rBV	414769	895368	77.90%	8.417%
25	6.063	1546	1562	1588	rBV	273900	585801	50.97%	5.507%
26	6.426	1673	1675	1679	rBV4	769	454	0.04%	0.004%
27	6.461	1683	1686	1691	rBV5	609	511	0.04%	0.005%
28	6.487	1691	1694	1696	rBV2	860	506	0.04%	0.005%
29	6.529	1703	1707	1711	rBV3	611	571	0.05%	0.005%
30	6.593	1723	1727	1728	rBV2	648	430	0.04%	0.004%
31	6.629	1735	1738	1740	rBV2	592	402	0.03%	0.004%
32	6.686	1753	1756	1760	rBV3	892	886	0.08%	0.008%
33	6.728	1766	1769	1775	rVB5	1267	1142	0.10%	0.011%
34	6.770	1778	1782	1783	rBV2	738	566	0.05%	0.005%
35	6.802	1790	1792	1797	rVB2	997	716	0.06%	0.007%
36	6.857	1805	1809	1811	rBV3	551	422	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027223.D
 Acq On : 05 Aug 2022 14:28
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.915	1826	1827	1831	rBV4	453	338	0.03%	0.003%
38	6.979	1837	1847	1878	rBV	124238	245676	21.37%	2.310%
39	7.191	1911	1913	1915	rBV3	859	408	0.04%	0.004%
40	7.310	1938	1950	1979	rBV	381159	705391	61.37%	6.631%
41	7.619	2037	2046	2071	rBV2	90981	168557	14.67%	1.585%
42	7.796	2096	2101	2102	rBV4	993	774	0.07%	0.007%
43	7.876	2124	2126	2133	rVB5	1080	691	0.06%	0.006%
44	7.915	2133	2138	2140	rBV3	665	581	0.05%	0.005%
45	7.973	2153	2156	2158	rBV3	721	380	0.03%	0.004%
46	7.989	2158	2161	2163	rVB2	735	349	0.03%	0.003%
47	7.998	2163	2164	2168	rBV3	944	423	0.04%	0.004%
48	8.021	2168	2171	2173	rBV3	504	299	0.03%	0.003%
49	8.085	2181	2191	2230	rBV	380729	770062	67.00%	7.239%
50	8.513	2320	2324	2325	rBV4	610	430	0.04%	0.004%
51	8.670	2368	2373	2376	rBV3	677	648	0.06%	0.006%
52	8.690	2376	2379	2381	rBV3	710	357	0.03%	0.003%
53	8.747	2394	2397	2400	rBV4	742	579	0.05%	0.005%
54	8.764	2400	2402	2406	rBV2	1102	645	0.06%	0.006%
55	8.847	2416	2428	2458	rBV	665295	1107714	96.38%	10.414%
56	9.204	2537	2539	2541	rBV3	753	353	0.03%	0.003%
57	9.487	2625	2627	2630	rBV2	426	356	0.03%	0.003%
58	9.567	2648	2652	2653	rVB2	703	334	0.03%	0.003%
59	9.577	2653	2655	2658	rVB	620	377	0.03%	0.004%
60	9.596	2658	2661	2662	rBV	585	309	0.03%	0.003%
61	9.622	2666	2669	2670	rBV	681	313	0.03%	0.003%
62	9.657	2677	2680	2683	rVB3	820	599	0.05%	0.006%
63	9.731	2701	2703	2707	rVB2	782	491	0.04%	0.005%
64	9.783	2714	2719	2721	rBV3	291	299	0.03%	0.003%
65	9.857	2740	2742	2744	rBV2	715	358	0.03%	0.003%
66	9.956	2770	2773	2776	rBV3	552	436	0.04%	0.004%
67	9.982	2778	2781	2785	rBV3	537	449	0.04%	0.004%
68	10.043	2796	2800	2801	rBV2	811	524	0.05%	0.005%
69	10.098	2814	2817	2820	rVB3	439	307	0.03%	0.003%
70	10.210	2841	2852	2872	rBV	462869	726935	63.25%	6.834%
71	10.329	2886	2889	2892	rBV5	530	360	0.03%	0.003%
72	10.390	2904	2908	2913	rVB4	677	691	0.06%	0.006%
73	10.532	2949	2952	2956	rVB2	669	501	0.04%	0.005%
74	10.657	2989	2991	2995	rBV3	702	449	0.04%	0.004%
75	10.693	2999	3002	3004	rBV2	708	439	0.04%	0.004%
76	10.728	3010	3013	3015	rBV2	834	405	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027223.D
 Acq On : 05 Aug 2022 14:28
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.780	3026	3029	3034	rVB5	534	478	0.04%	0.004%
78	10.828	3036	3044	3047	rBV2	683	802	0.07%	0.008%
79	10.915	3070	3071	3075	rVB2	702	413	0.04%	0.004%
80	10.969	3084	3088	3090	rBV3	659	476	0.04%	0.004%
81	10.998	3095	3097	3098	rBV	901	402	0.03%	0.004%
82	11.030	3104	3107	3109	rBV2	877	639	0.06%	0.006%
83	11.075	3114	3121	3123	rBV4	821	774	0.07%	0.007%
84	11.194	3155	3158	3161	rBV3	649	375	0.03%	0.004%
85	11.246	3162	3174	3194	rBV	580006	896728	78.02%	8.430%
86	11.622	3276	3291	3313	rBV	515293	825203	71.80%	7.758%
87	12.304	3499	3503	3504	rBV2	664	455	0.04%	0.004%
88	12.352	3515	3518	3519	rBV2	641	323	0.03%	0.003%
89	12.439	3544	3545	3548	rVB3	862	340	0.03%	0.003%
90	12.561	3578	3583	3589	rBV5	1051	1339	0.12%	0.013%
91	12.866	3676	3678	3680	rBV2	686	474	0.04%	0.004%
92	12.940	3698	3701	3705	rVB2	762	379	0.03%	0.004%
93	13.123	3754	3758	3759	rBV	635	440	0.04%	0.004%
94	13.461	3860	3863	3867	rVB2	1176	777	0.07%	0.007%
95	13.480	3867	3869	3870	rBV	831	378	0.03%	0.004%
96	13.503	3874	3876	3880	rVV3	632	385	0.03%	0.004%
97	13.519	3880	3881	3886	rVV4	468	329	0.03%	0.003%
98	13.956	4013	4017	4019	rBV4	992	666	0.06%	0.006%
99	14.123	4067	4069	4073	rBV4	642	403	0.04%	0.004%
100	15.667	4546	4549	4555	rVB	10077	5997	0.52%	0.056%




Sum of corrected areas: 10637133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027223.D
Acq On : 05 Aug 2022 14:28
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

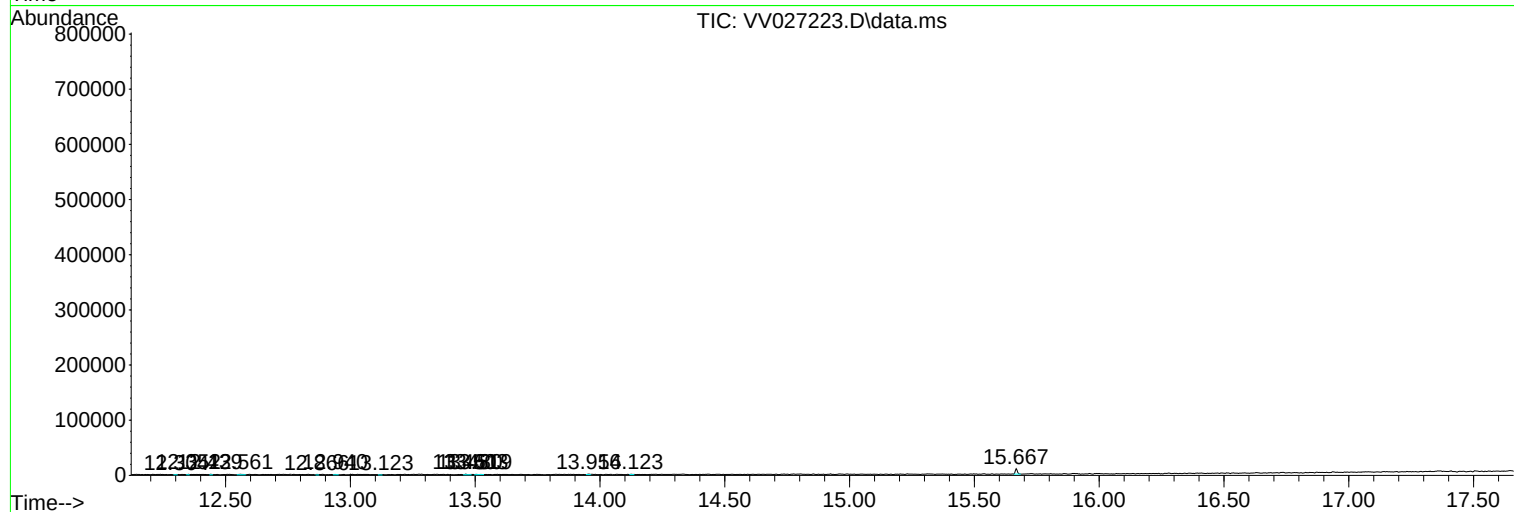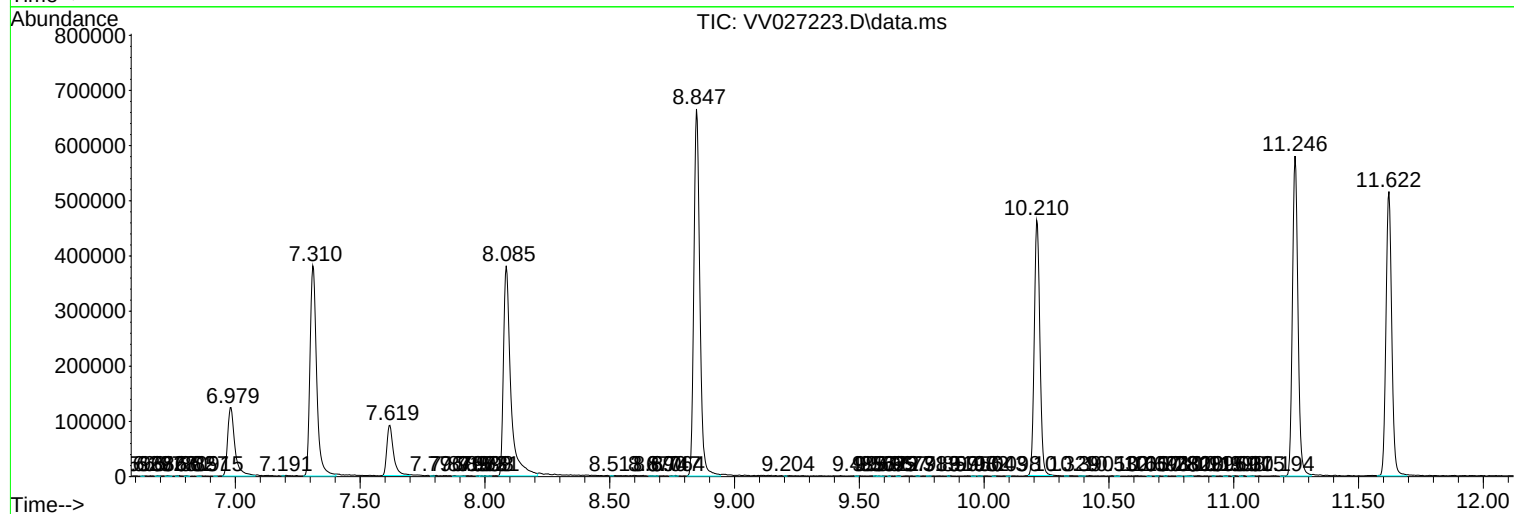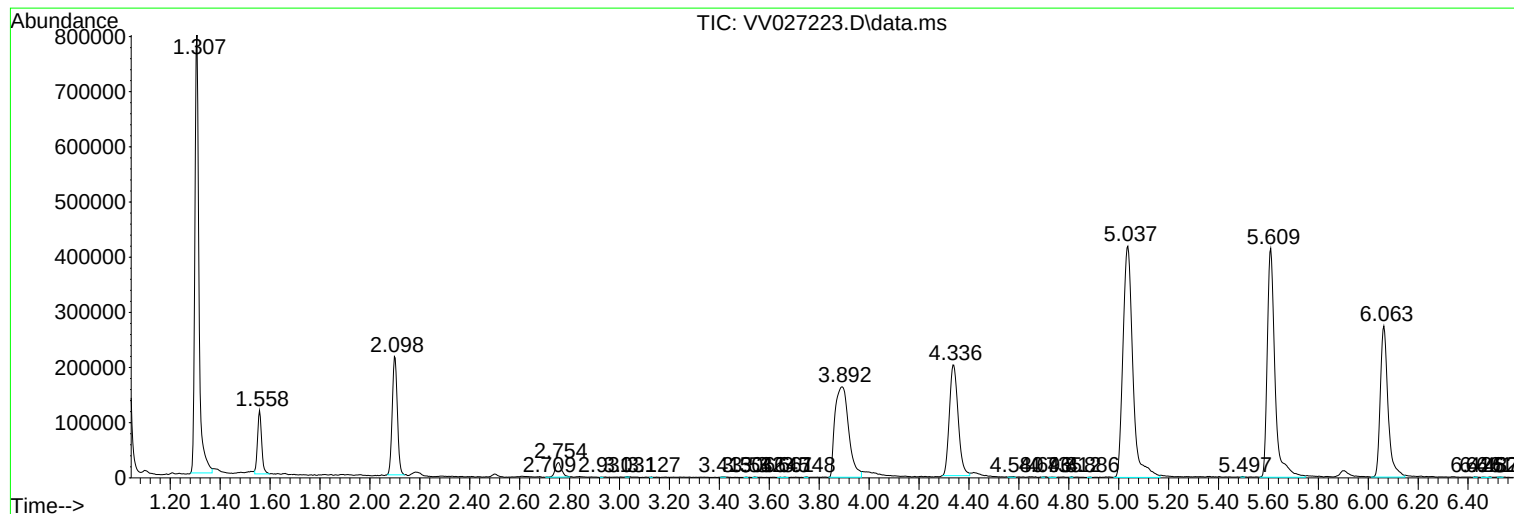

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027223.D
Acq On : 05 Aug 2022 14:28
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027223.D
Acq On : 05 Aug 2022 14:28
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------