

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027224.D
 Acq On : 05 Aug 2022 14:53
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	119139	130752	11.33%	1.217%
2	1.561	155	162	172	rVB	109915	128940	11.18%	1.200%
3	2.101	322	330	342	rVB	200996	276484	23.97%	2.572%
4	2.754	520	533	555	rBV	670299	1153616	100.00%	10.733%
5	3.124	646	648	650	rBV3	682	415	0.04%	0.004%
6	3.162	656	660	662	rBV3	625	478	0.04%	0.004%
7	3.175	662	664	668	rVV4	694	445	0.04%	0.004%
8	3.330	710	712	715	rVV2	531	229	0.02%	0.002%
9	3.343	715	716	719	rVB	542	173	0.01%	0.002%
10	3.384	727	729	737	rVB3	665	631	0.05%	0.006%
11	3.426	737	742	743	rBV2	663	532	0.05%	0.005%
12	3.461	751	753	755	rBV2	511	266	0.02%	0.002%
13	3.478	755	758	763	rVB4	889	673	0.06%	0.006%
14	3.506	763	767	769	rBV2	512	432	0.04%	0.004%
15	3.548	778	780	782	rBV3	488	259	0.02%	0.002%
16	3.577	785	789	791	rBV3	610	508	0.04%	0.005%
17	3.606	794	798	800	rBV3	524	410	0.04%	0.004%
18	3.706	828	829	831	rBV	586	240	0.02%	0.002%
19	3.757	843	845	852	rVB4	856	688	0.06%	0.006%
20	3.802	857	859	862	rBV2	615	281	0.02%	0.003%
21	3.834	867	869	871	rBV2	723	430	0.04%	0.004%
22	3.902	872	890	914	rBV2	277938	922240	79.94%	8.581%
23	4.342	1011	1027	1048	rBV	192055	476527	41.31%	4.434%
24	4.822	1174	1176	1178	rBV2	537	238	0.02%	0.002%
25	4.941	1209	1213	1216	rBV4	607	471	0.04%	0.004%
26	4.953	1216	1217	1219	rBV	488	173	0.01%	0.002%
27	5.040	1228	1244	1265	rBV2	398621	1043456	90.45%	9.709%
28	5.326	1331	1333	1338	rBV5	1054	822	0.07%	0.008%
29	5.445	1367	1370	1371	rVB2	565	265	0.02%	0.002%
30	5.484	1381	1382	1383	rBV	456	127	0.01%	0.001%
31	5.522	1392	1394	1397	rBV4	509	358	0.03%	0.003%
32	5.545	1397	1401	1404	rBV4	968	722	0.06%	0.007%
33	5.613	1409	1422	1438	rBV	392021	789345	68.42%	7.344%
34	5.912	1503	1515	1534	rBV5	39521	94836	8.22%	0.882%
35	6.066	1551	1563	1593	rBV	261167	557137	48.29%	5.184%
36	6.403	1666	1668	1669	rBV2	422	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027224.D
 Acq On : 05 Aug 2022 14:53
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.535	1707	1709	1710	rBV2	477	248	0.02%	0.002%
38	6.641	1739	1742	1743	rBV3	442	317	0.03%	0.003%
39	6.715	1764	1765	1771	rVB4	1041	623	0.05%	0.006%
40	6.886	1816	1818	1820	rBV2	599	284	0.02%	0.003%
41	6.908	1823	1825	1828	rVB3	466	205	0.02%	0.002%
42	6.924	1828	1830	1833	rBV3	649	288	0.02%	0.003%
43	6.947	1833	1837	1838	rBV3	464	346	0.03%	0.003%
44	6.985	1838	1849	1878	rBV	114218	230454	19.98%	2.144%
45	7.313	1939	1951	1976	rBV	359056	655221	56.80%	6.096%
46	7.619	2037	2046	2071	rBV	85636	159400	13.82%	1.483%
47	7.921	2137	2140	2144	rBV4	522	401	0.03%	0.004%
48	7.969	2153	2155	2156	rBV2	584	231	0.02%	0.002%
49	8.024	2169	2172	2177	rVB5	613	545	0.05%	0.005%
50	8.088	2180	2192	2224	rBV	387572	772798	66.99%	7.190%
51	8.625	2357	2359	2364	rVB5	772	478	0.04%	0.004%
52	8.850	2418	2429	2456	rBV	633782	1033802	89.61%	9.619%
53	9.300	2567	2569	2570	rBV	576	190	0.02%	0.002%
54	9.310	2570	2572	2574	rVV3	559	238	0.02%	0.002%
55	9.477	2621	2624	2626	rBV3	529	331	0.03%	0.003%
56	9.622	2667	2669	2674	rVB3	829	527	0.05%	0.005%
57	9.683	2683	2688	2693	rBV5	872	1108	0.10%	0.010%
58	9.741	2704	2706	2709	rVB2	695	352	0.03%	0.003%
59	9.786	2718	2720	2723	rBV2	953	589	0.05%	0.005%
60	9.834	2731	2735	2739	rBV3	703	666	0.06%	0.006%
61	9.863	2743	2744	2745	rBV3	525	194	0.02%	0.002%
62	9.908	2756	2758	2759	rBV3	446	194	0.02%	0.002%
63	9.931	2763	2765	2766	rBV	629	305	0.03%	0.003%
64	9.985	2780	2782	2786	rVB3	763	445	0.04%	0.004%
65	10.011	2788	2790	2792	rBV	688	267	0.02%	0.002%
66	10.024	2792	2794	2796	rBV3	484	154	0.01%	0.001%
67	10.050	2799	2802	2803	rBV2	596	343	0.03%	0.003%
68	10.095	2814	2816	2819	rVB3	530	279	0.02%	0.003%
69	10.111	2819	2821	2822	rBV	474	203	0.02%	0.002%
70	10.156	2832	2835	2837	rBV	636	356	0.03%	0.003%
71	10.214	2840	2853	2872	rBV	454508	711467	61.67%	6.620%
72	10.542	2953	2955	2958	rBV4	583	406	0.04%	0.004%
73	10.654	2988	2990	2992	rBV2	509	209	0.02%	0.002%
74	10.706	3004	3006	3008	rBV3	721	448	0.04%	0.004%
75	10.722	3008	3011	3015	rVV	896	655	0.06%	0.006%
76	10.741	3015	3017	3021	rVB4	475	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027224.D
 Acq On : 05 Aug 2022 14:53
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.808	3036	3038	3040	rBV3	824	480	0.04%	0.004%
78	10.931	3072	3076	3082	rVB5	695	640	0.06%	0.006%
79	10.995	3092	3096	3100	rBV2	491	464	0.04%	0.004%
80	11.066	3117	3118	3123	rBV2	787	357	0.03%	0.003%
81	11.095	3125	3127	3132	rVB2	728	600	0.05%	0.006%
82	11.117	3132	3134	3135	rBV2	607	291	0.03%	0.003%
83	11.178	3149	3153	3156	rBV3	595	414	0.04%	0.004%
84	11.194	3156	3158	3162	rBV4	743	399	0.03%	0.004%
85	11.246	3164	3174	3199	rBV	520158	818784	70.98%	7.618%
86	11.577	3275	3277	3279	rBV2	711	358	0.03%	0.003%
87	11.622	3280	3291	3313	rVV	487600	758824	65.78%	7.060%
88	11.789	3340	3343	3344	rBV2	744	364	0.03%	0.003%
89	11.956	3393	3395	3397	rBV2	768	345	0.03%	0.003%
90	12.133	3448	3450	3454	rBV3	679	342	0.03%	0.003%
91	12.435	3542	3544	3545	rBV	859	339	0.03%	0.003%
92	12.471	3553	3555	3559	rBV2	683	405	0.04%	0.004%
93	12.863	3675	3677	3680	rBV3	832	557	0.05%	0.005%
94	12.889	3680	3685	3691	rVV7	978	1304	0.11%	0.012%
95	13.159	3766	3769	3771	rBV3	776	319	0.03%	0.003%
96	13.307	3813	3815	3818	rBV3	1039	562	0.05%	0.005%
97	13.496	3871	3874	3876	rBV2	1001	615	0.05%	0.006%
98	13.606	3905	3908	3910	rBV2	643	422	0.04%	0.004%
99	13.654	3921	3923	3925	rBV2	793	449	0.04%	0.004%
100	15.172	4393	4395	4398	rBV4	912	625	0.05%	0.006%




Sum of corrected areas: 10747813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027224.D
Acq On : 05 Aug 2022 14:53
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

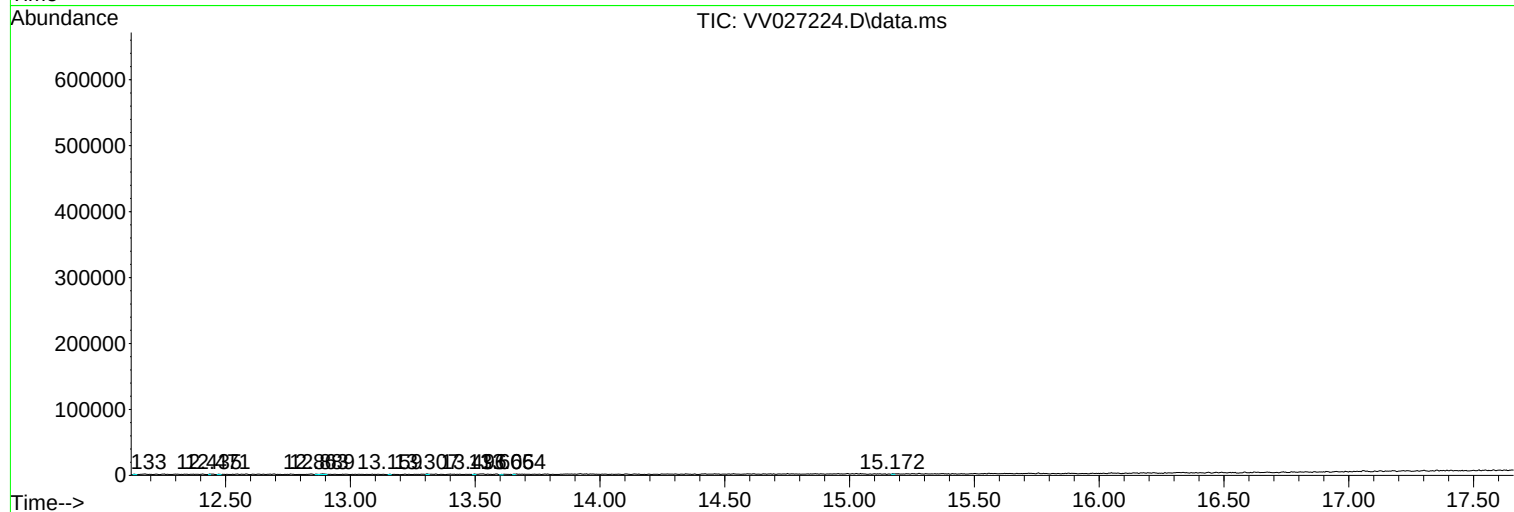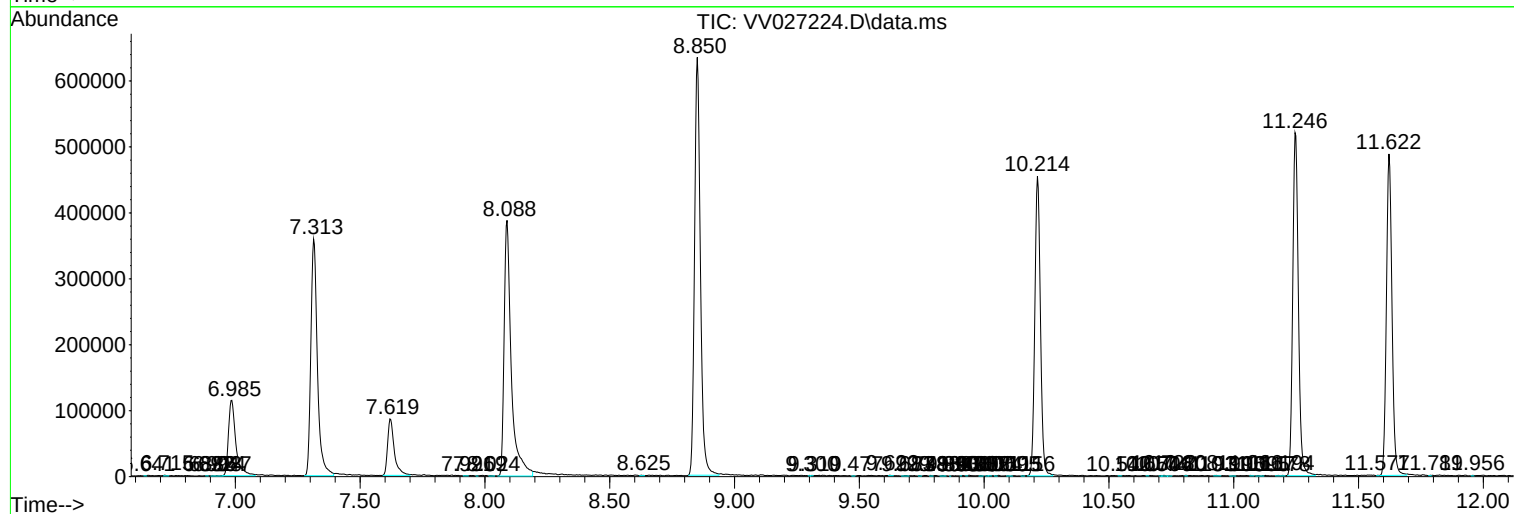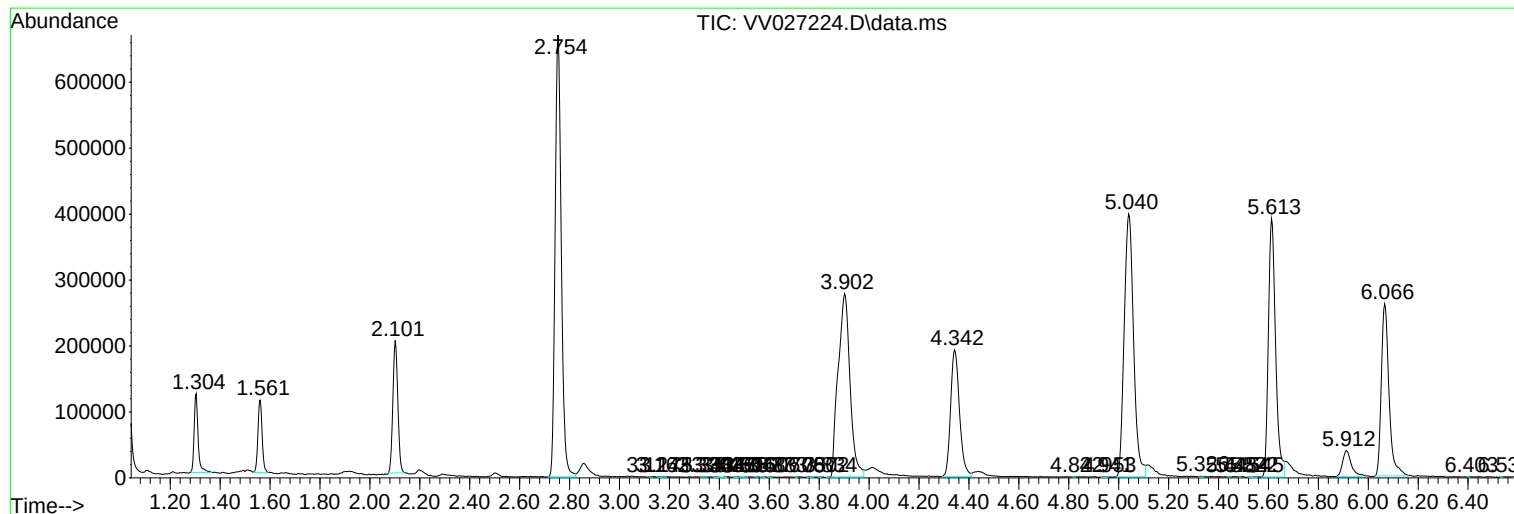

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027224.D
Acq On : 05 Aug 2022 14:53
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027224.D
Acq On : 05 Aug 2022 14:53
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc