

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027225.D
 Acq On : 05 Aug 2022 15:18
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	107	rVB	120665	135990	12.92%	1.281%
2	1.558	155	161	177	rVB	114576	136301	12.95%	1.284%
3	2.101	321	330	343	rBV	201989	286028	27.18%	2.695%
4	2.458	439	441	446	rBV5	668	630	0.06%	0.006%
5	2.503	448	455	468	rVB3	8088	13684	1.30%	0.129%
6	2.754	521	533	555	rBV	526216	910990	86.55%	8.584%
7	3.191	662	669	670	rBV5	630	652	0.06%	0.006%
8	3.233	679	682	683	rBV2	576	318	0.03%	0.003%
9	3.349	715	718	720	rBV3	802	464	0.04%	0.004%
10	3.384	727	729	731	rBV2	710	358	0.03%	0.003%
11	3.436	740	745	746	rBV2	755	422	0.04%	0.004%
12	3.465	750	754	756	rVB4	650	390	0.04%	0.004%
13	3.487	756	761	764	rVB5	706	493	0.05%	0.005%
14	3.526	771	773	775	rBV	588	326	0.03%	0.003%
15	3.542	775	778	783	rVB3	515	398	0.04%	0.004%
16	3.619	797	802	806	rBV4	535	608	0.06%	0.006%
17	3.725	832	835	837	rBV3	632	353	0.03%	0.003%
18	3.790	853	855	860	rVV5	779	551	0.05%	0.005%
19	3.902	872	890	916	rBV3	305473	1000187	95.03%	9.424%
20	4.343	1013	1027	1049	rBV	189993	471178	44.77%	4.440%
21	4.600	1104	1107	1110	rBV4	1189	760	0.07%	0.007%
22	4.770	1156	1160	1162	rBV5	790	502	0.05%	0.005%
23	4.892	1194	1198	1200	rBV3	846	563	0.05%	0.005%
24	4.908	1200	1203	1207	rVB3	752	562	0.05%	0.005%
25	5.040	1225	1244	1263	rBV2	401070	1052532	100.00%	9.918%
26	5.474	1375	1379	1382	rBV4	706	641	0.06%	0.006%
27	5.571	1406	1409	1410	rBV2	658	341	0.03%	0.003%
28	5.613	1410	1422	1438	rBV	395286	798947	75.91%	7.528%
29	5.854	1494	1497	1501	rBV5	916	827	0.08%	0.008%
30	5.908	1506	1514	1524	rVV9	10064	21702	2.06%	0.204%
31	6.021	1547	1549	1550	rBV2	1033	445	0.04%	0.004%
32	6.066	1550	1563	1595	rVV	263334	561592	53.36%	5.292%
33	6.323	1640	1643	1645	rBV3	595	447	0.04%	0.004%
34	6.362	1654	1655	1661	rVB4	808	514	0.05%	0.005%
35	6.387	1661	1663	1666	rVV2	692	393	0.04%	0.004%
36	6.535	1707	1709	1712	rVB3	1029	519	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027225.D
 Acq On : 05 Aug 2022 15:18
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.777	1778	1784	1789	rBV4	873	797	0.08%	0.008%
38	6.799	1789	1791	1794	rBV3	492	328	0.03%	0.003%
39	6.834	1798	1802	1805	rVB4	909	669	0.06%	0.006%
40	6.867	1808	1812	1815	rBV4	821	708	0.07%	0.007%
41	6.921	1826	1829	1831	rBV3	584	334	0.03%	0.003%
42	6.941	1831	1835	1837	rVB4	790	519	0.05%	0.005%
43	6.986	1837	1849	1876	rBV	116973	233572	22.19%	2.201%
44	7.313	1940	1951	1985	rBV	363991	664079	63.09%	6.257%
45	7.619	2037	2046	2064	rBV2	85538	157605	14.97%	1.485%
46	7.751	2085	2087	2091	rBV4	928	741	0.07%	0.007%
47	7.899	2132	2133	2135	rBV2	673	338	0.03%	0.003%
48	8.088	2179	2192	2230	rBV	387439	773935	73.53%	7.293%
49	8.616	2354	2356	2359	rBV3	980	550	0.05%	0.005%
50	8.632	2359	2361	2363	rBV	827	346	0.03%	0.003%
51	8.728	2388	2391	2393	rBV3	814	401	0.04%	0.004%
52	8.850	2418	2429	2449	rBV	629259	1035053	98.34%	9.753%
53	9.313	2571	2573	2577	rVB4	863	480	0.05%	0.005%
54	9.346	2581	2583	2586	rVB	560	333	0.03%	0.003%
55	9.375	2586	2592	2597	rBV8	1212	1738	0.17%	0.016%
56	9.426	2605	2608	2609	rBV2	729	469	0.04%	0.004%
57	9.477	2621	2624	2626	rVV3	677	301	0.03%	0.003%
58	9.529	2637	2640	2641	rVB2	712	336	0.03%	0.003%
59	9.548	2643	2646	2648	rBV3	840	487	0.05%	0.005%
60	9.561	2648	2650	2653	rVB2	528	316	0.03%	0.003%
61	9.580	2653	2656	2659	rBV3	848	673	0.06%	0.006%
62	9.603	2659	2663	2664	rBV2	924	534	0.05%	0.005%
63	9.780	2716	2718	2722	rVB4	579	403	0.04%	0.004%
64	9.805	2722	2726	2728	rBV5	918	690	0.07%	0.007%
65	9.825	2730	2732	2735	rVV2	1100	626	0.06%	0.006%
66	9.895	2752	2754	2757	rBV2	662	434	0.04%	0.004%
67	9.985	2778	2782	2784	rBV3	582	348	0.03%	0.003%
68	10.001	2784	2787	2788	rVV2	671	359	0.03%	0.003%
69	10.030	2791	2796	2798	rBV3	520	403	0.04%	0.004%
70	10.214	2841	2853	2875	rBV	455084	710363	67.49%	6.694%
71	10.426	2916	2919	2921	rVV3	698	415	0.04%	0.004%
72	10.548	2952	2957	2958	rBV2	769	523	0.05%	0.005%
73	10.596	2970	2972	2976	rVB4	535	311	0.03%	0.003%
74	10.841	3046	3048	3050	rBV2	1040	539	0.05%	0.005%
75	10.956	3082	3084	3087	rVV3	812	544	0.05%	0.005%
76	10.998	3093	3097	3099	rBV5	477	341	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027225.D
 Acq On : 05 Aug 2022 15:18
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.175	3149	3152	3154	rVB3	528	342	0.03%	0.003%
78	11.191	3154	3157	3162	rBV4	916	904	0.09%	0.009%
79	11.249	3163	3175	3198	rBV	522491	820747	77.98%	7.734%
80	11.381	3214	3216	3221	rBV5	917	669	0.06%	0.006%
81	11.622	3280	3291	3307	rBV	476433	759784	72.19%	7.159%
82	11.944	3389	3391	3394	rBV3	513	361	0.03%	0.003%
83	11.995	3402	3407	3408	rBV3	836	706	0.07%	0.007%
84	12.114	3441	3444	3449	rBV6	1094	1180	0.11%	0.011%
85	12.191	3466	3468	3472	rVB2	742	394	0.04%	0.004%
86	12.365	3516	3522	3532	rVB8	4444	7062	0.67%	0.067%
87	12.718	3629	3632	3633	rBV2	677	422	0.04%	0.004%
88	12.879	3678	3682	3684	rBV4	2546	2069	0.20%	0.019%
89	12.953	3699	3705	3711	rVB7	3474	3779	0.36%	0.036%
90	13.056	3728	3737	3749	rBV10	5345	10218	0.97%	0.096%
91	13.156	3766	3768	3771	rBV4	777	591	0.06%	0.006%
92	13.304	3812	3814	3818	rVB4	693	358	0.03%	0.003%
93	13.461	3859	3863	3866	rBV4	660	564	0.05%	0.005%
94	13.500	3866	3875	3878	rBV9	3755	5470	0.52%	0.052%
95	13.599	3905	3906	3909	rVB3	922	356	0.03%	0.003%
96	13.818	3971	3974	3976	rBV3	766	550	0.05%	0.005%
97	13.857	3984	3986	3987	rBV	828	409	0.04%	0.004%
98	13.982	4023	4025	4029	rVB4	1269	817	0.08%	0.008%
99	14.005	4029	4032	4035	rBV2	962	676	0.06%	0.006%
100	14.024	4035	4038	4040	rBV4	901	694	0.07%	0.007%




Sum of corrected areas: 10612671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027225.D
Acq On : 05 Aug 2022 15:18
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

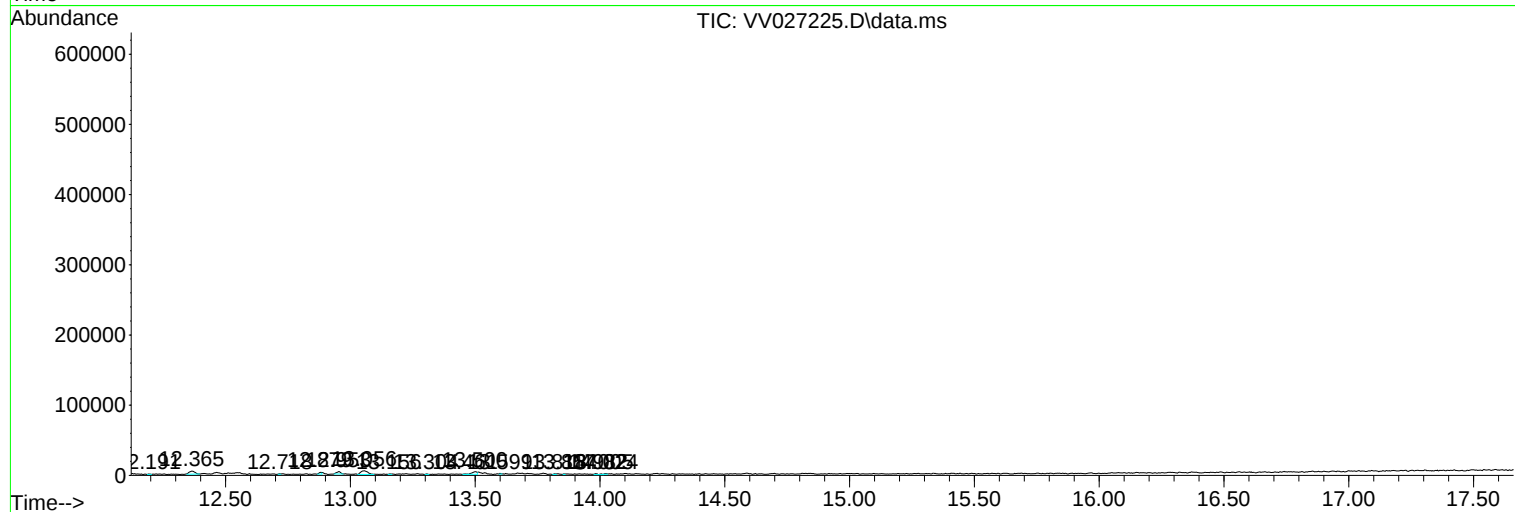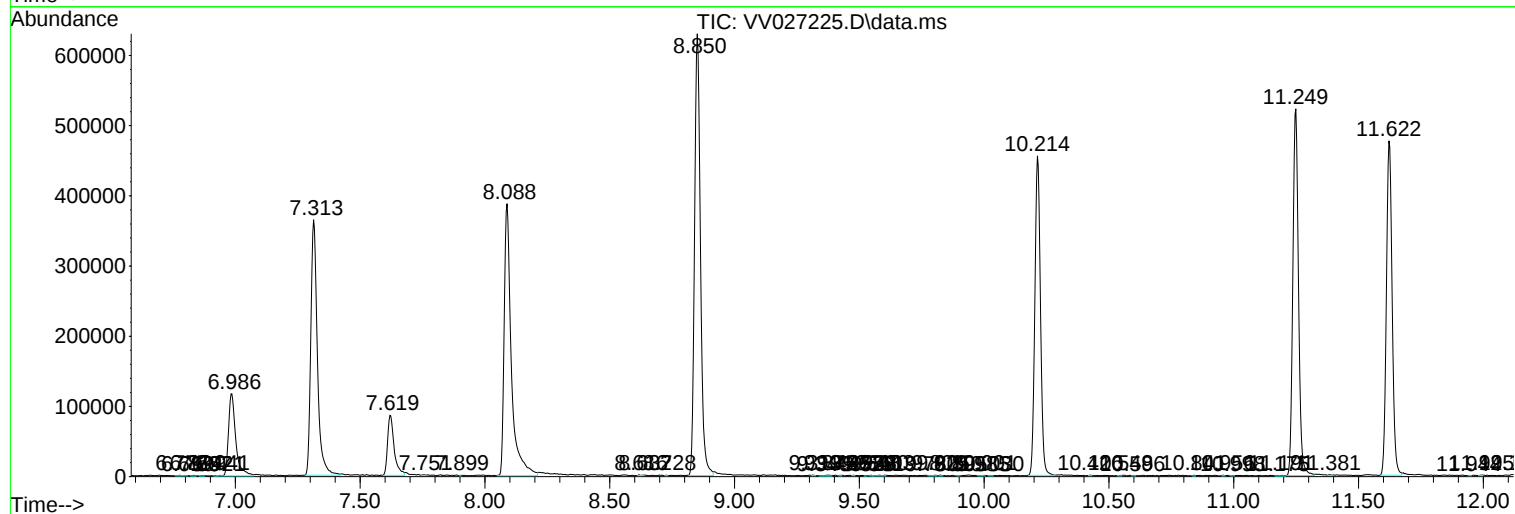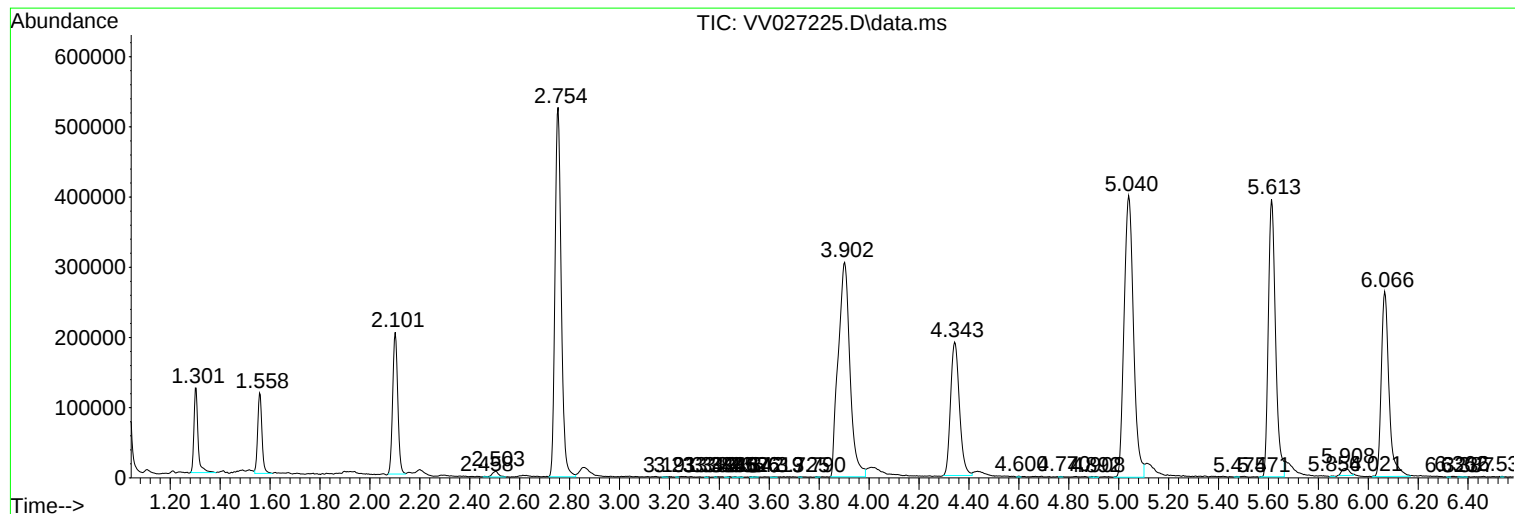

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027225.D
Acq On : 05 Aug 2022 15:18
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027225.D
Acq On : 05 Aug 2022 15:18
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------