

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V080522\
 Data File : VV027226.D
 Acq On : 05 Aug 2022 15:42
 Operator : SY/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rBV	227433	253581	14.76%	1.930%
2	1.558	155	161	177	rVB	176527	207446	12.07%	1.579%
3	2.101	320	330	342	rBV	372750	530986	30.90%	4.041%
4	2.477	443	447	448	rBV2	1049	686	0.04%	0.005%
5	2.558	466	472	477	rBV6	1093	1366	0.08%	0.010%
6	2.754	523	533	550	rBV	37227	68582	3.99%	0.522%
7	2.960	595	597	600	rBV2	609	373	0.02%	0.003%
8	2.992	605	607	610	rVB3	747	418	0.02%	0.003%
9	3.156	656	658	660	rBV	367	198	0.01%	0.002%
10	3.194	668	670	673	rVB2	524	287	0.02%	0.002%
11	3.214	673	676	678	rVB3	590	381	0.02%	0.003%
12	3.230	678	681	683	rBV4	600	401	0.02%	0.003%
13	3.333	709	713	714	rBV3	504	260	0.02%	0.002%
14	3.371	721	725	727	rBV2	776	607	0.04%	0.005%
15	3.410	734	737	738	rBV	545	327	0.02%	0.002%
16	3.506	765	767	772	rVB3	653	335	0.02%	0.003%
17	3.657	808	814	816	rBV3	726	617	0.04%	0.005%
18	3.722	831	834	839	rBV4	708	757	0.04%	0.006%
19	3.757	842	845	847	rBV2	448	218	0.01%	0.002%
20	3.834	866	869	870	rBV2	847	341	0.02%	0.003%
21	3.902	870	890	912	rBV2	596529	1718599	100.00%	13.080%
22	4.342	1010	1027	1049	rBV	253677	649358	37.78%	4.942%
23	4.960	1217	1219	1224	rBV3	661	481	0.03%	0.004%
24	5.040	1228	1244	1264	rBV2	614156	1586621	92.32%	12.075%
25	5.294	1321	1323	1328	rVB7	1751	1043	0.06%	0.008%
26	5.490	1380	1384	1387	rBV3	802	679	0.04%	0.005%
27	5.612	1410	1422	1459	rBV	374517	794172	46.21%	6.044%
28	5.911	1500	1515	1541	rBV2	168338	367381	21.38%	2.796%
29	6.066	1550	1563	1594	rBV	365034	768507	44.72%	5.849%
30	6.471	1687	1689	1692	rVV5	565	364	0.02%	0.003%
31	6.532	1705	1708	1710	rBV3	1055	674	0.04%	0.005%
32	6.693	1756	1758	1759	rBV2	691	218	0.01%	0.002%
33	6.725	1766	1768	1771	rBV2	515	328	0.02%	0.002%
34	6.828	1798	1800	1802	rVB3	692	237	0.01%	0.002%
35	6.882	1815	1817	1819	rVV3	521	267	0.02%	0.002%
36	6.918	1826	1828	1829	rBV2	617	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW080522\
 Data File : VW027226.D
 Acq On : 05 Aug 2022 15:42
 Operator : SY/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.982	1837	1848	1878	rBV	171670	330711	19.24%	2.517%
38	7.313	1939	1951	1983	rBV	641134	1167259	67.92%	8.884%
39	7.619	2036	2046	2072	rBV	123054	229276	13.34%	1.745%
40	7.905	2132	2135	2139	rBV3	991	748	0.04%	0.006%
41	7.937	2143	2145	2149	rBV3	914	673	0.04%	0.005%
42	7.976	2149	2157	2170	rBV6	10065	18249	1.06%	0.139%
43	8.088	2182	2192	2223	rBV	420220	838689	48.80%	6.383%
44	8.580	2343	2345	2346	rBV2	570	210	0.01%	0.002%
45	8.609	2350	2354	2356	rBV3	1267	853	0.05%	0.006%
46	8.850	2418	2429	2456	rBV	598255	996014	57.95%	7.580%
47	9.066	2494	2496	2499	rBV3	1088	642	0.04%	0.005%
48	9.326	2575	2577	2582	rBV4	1018	813	0.05%	0.006%
49	9.480	2621	2625	2630	rBV4	912	857	0.05%	0.007%
50	9.535	2640	2642	2644	rVB2	540	230	0.01%	0.002%
51	9.554	2646	2648	2649	rBV2	558	212	0.01%	0.002%
52	9.596	2658	2661	2663	rBV	728	400	0.02%	0.003%
53	9.622	2667	2669	2670	rBV2	492	204	0.01%	0.002%
54	9.725	2699	2701	2703	rVB2	487	188	0.01%	0.001%
55	9.860	2741	2743	2745	rVB3	942	338	0.02%	0.003%
56	9.873	2745	2747	2750	rBV3	626	397	0.02%	0.003%
57	9.924	2761	2763	2765	rVB2	794	282	0.02%	0.002%
58	9.995	2781	2785	2788	rVB4	563	409	0.02%	0.003%
59	10.014	2788	2791	2792	rBV3	870	438	0.03%	0.003%
60	10.040	2797	2799	2803	rVB3	1577	764	0.04%	0.006%
61	10.059	2803	2805	2807	rBV	542	339	0.02%	0.003%
62	10.117	2821	2823	2828	rVB3	953	575	0.03%	0.004%
63	10.143	2828	2831	2836	rBV3	834	807	0.05%	0.006%
64	10.213	2841	2853	2879	rVV	505680	802639	46.70%	6.109%
65	10.390	2906	2908	2911	rBV2	734	495	0.03%	0.004%
66	10.467	2931	2932	2934	rBV2	744	313	0.02%	0.002%
67	10.496	2939	2941	2945	rVB3	703	475	0.03%	0.004%
68	10.516	2945	2947	2949	rBV3	574	308	0.02%	0.002%
69	10.577	2961	2966	2968	rBV5	938	848	0.05%	0.006%
70	10.635	2981	2984	2986	rBV3	793	438	0.03%	0.003%
71	10.683	2997	2999	3001	rBV	569	337	0.02%	0.003%
72	10.728	3011	3013	3019	rVB4	794	496	0.03%	0.004%
73	10.757	3019	3022	3024	rBV2	538	347	0.02%	0.003%
74	10.776	3026	3028	3031	rVV2	714	383	0.02%	0.003%
75	10.840	3045	3048	3049	rBV2	1063	569	0.03%	0.004%
76	10.953	3080	3083	3084	rBV2	515	308	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027226.D
 Acq On : 05 Aug 2022 15:42
 Operator : SY/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.972	3087	3089	3092	rVV2	711	411	0.02%	0.003%
78	11.188	3148	3156	3158	rBV5	853	941	0.05%	0.007%
79	11.201	3158	3160	3161	rBV2	539	230	0.01%	0.002%
80	11.249	3163	3175	3197	rBV	510496	792097	46.09%	6.028%
81	11.500	3250	3253	3257	rBV4	617	644	0.04%	0.005%
82	11.622	3280	3291	3310	rBV	627806	979704	57.01%	7.456%
83	12.136	3449	3451	3455	rBV3	649	553	0.03%	0.004%
84	12.387	3527	3529	3531	rBV2	1163	471	0.03%	0.004%
85	12.432	3541	3543	3547	rBV3	662	508	0.03%	0.004%
86	12.480	3556	3558	3561	rBV3	740	326	0.02%	0.002%
87	12.545	3575	3578	3581	rBV2	1126	901	0.05%	0.007%
88	12.834	3666	3668	3670	rBV3	586	304	0.02%	0.002%
89	13.033	3728	3730	3733	rBV	811	501	0.03%	0.004%
90	13.120	3755	3757	3759	rBV2	583	273	0.02%	0.002%
91	13.181	3774	3776	3778	rBV	560	332	0.02%	0.003%
92	13.381	3835	3838	3842	rVB5	858	667	0.04%	0.005%
93	13.406	3844	3846	3849	rBV3	622	422	0.02%	0.003%
94	13.599	3904	3906	3909	rBV2	594	459	0.03%	0.003%
95	14.046	4041	4045	4047	rBV4	1215	1011	0.06%	0.008%
96	14.252	4106	4109	4110	rBV2	720	425	0.02%	0.003%
97	14.393	4151	4153	4154	rBV2	1154	541	0.03%	0.004%
98	14.567	4205	4207	4210	rBV3	866	638	0.04%	0.005%
99	15.413	4468	4470	4472	rBV2	868	416	0.02%	0.003%
100	15.554	4510	4514	4515	rBV3	1231	927	0.05%	0.007%




Sum of corrected areas: 13139608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027226.D
Acq On : 05 Aug 2022 15:42
Operator : SY/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

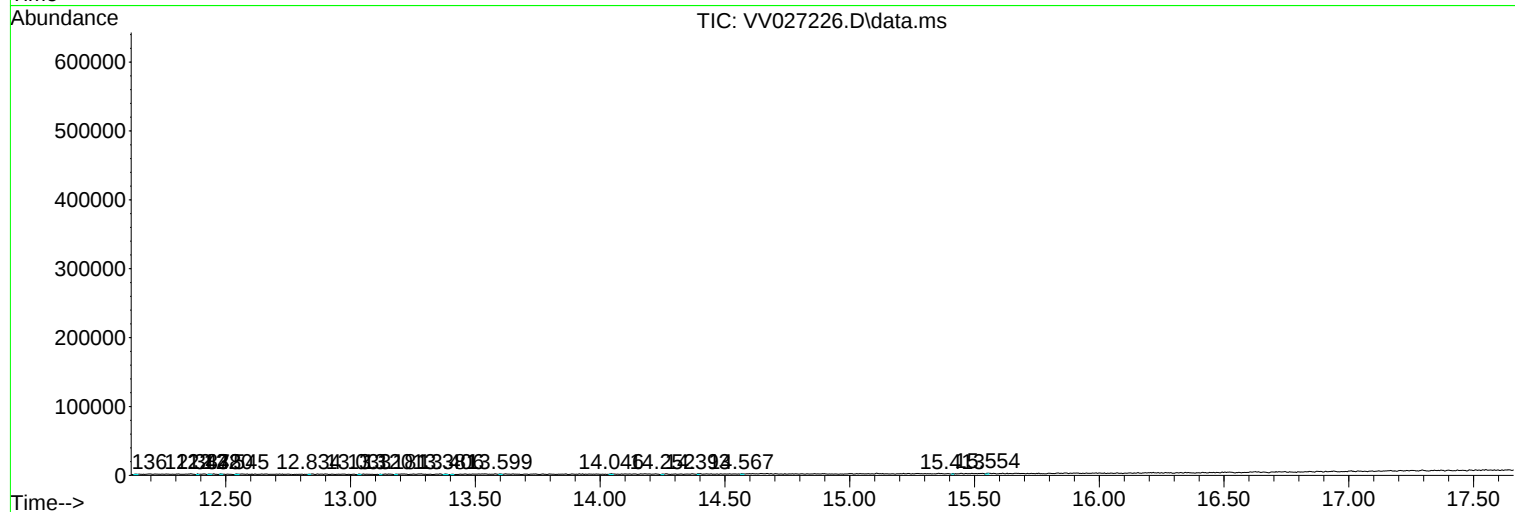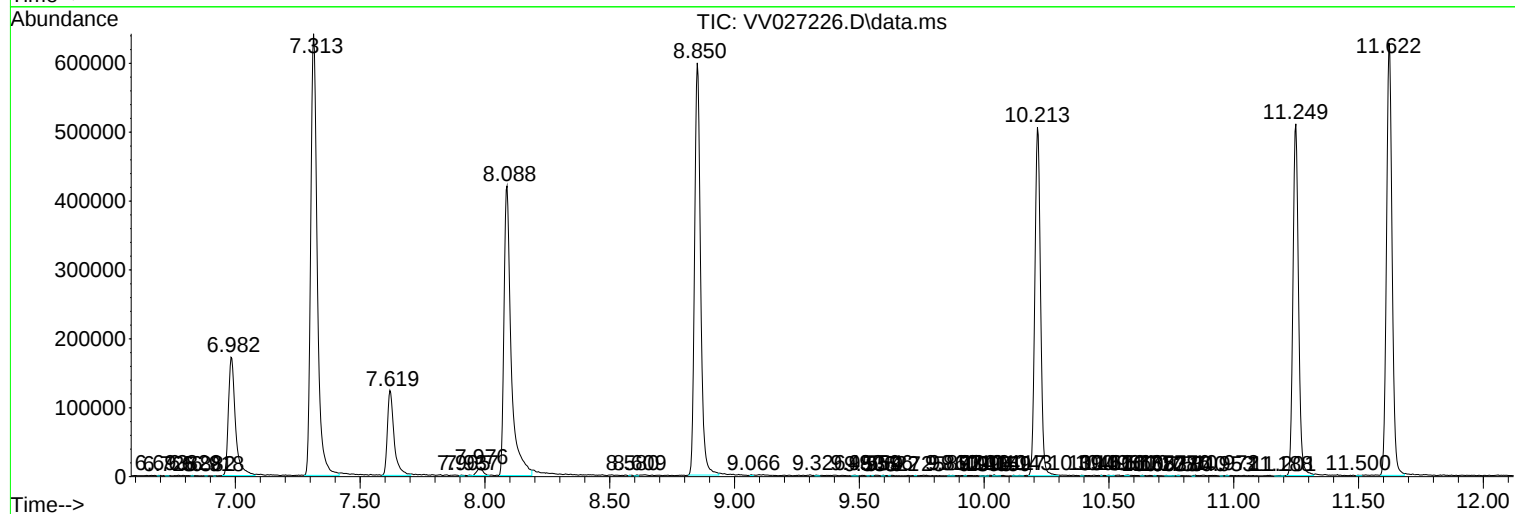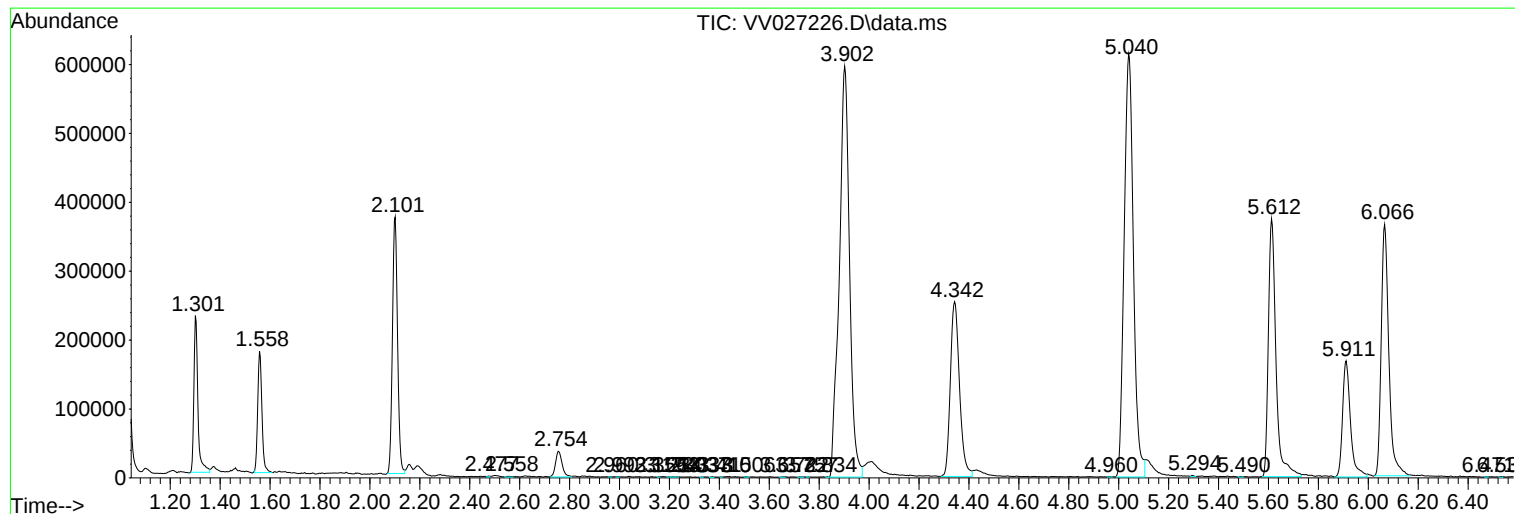

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027226.D
Acq On : 05 Aug 2022 15:42
Operator : SY/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027226.D
Acq On : 05 Aug 2022 15:42
Operator : SY/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------