

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V080522\
 Data File : VV027227.D
 Acq On : 05 Aug 2022 16:07
 Operator : SY/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	117	rVB	234436	275155	4.68%	1.520%
2	1.558	155	161	179	rVB	171292	206354	3.51%	1.140%
3	2.101	321	330	343	rVB	360030	506627	8.61%	2.799%
4	2.333	399	402	404	rBV4	1225	788	0.01%	0.004%
5	2.346	404	406	413	rVB6	1412	1323	0.02%	0.007%
6	2.561	471	473	476	rVB3	641	249	0.00%	0.001%
7	2.686	510	512	515	rBV2	713	304	0.01%	0.002%
8	2.712	515	520	521	rBV4	814	642	0.01%	0.004%
9	2.754	522	533	550	rVV	89006	156209	2.65%	0.863%
10	2.944	591	592	594	rBV2	622	231	0.00%	0.001%
11	2.992	605	607	610	rBV3	693	486	0.01%	0.003%
12	3.111	642	644	646	rVB3	570	252	0.00%	0.001%
13	3.137	649	652	655	rVB4	942	471	0.01%	0.003%
14	3.159	657	659	663	rVB3	794	477	0.01%	0.003%
15	3.297	699	702	704	rBV2	938	531	0.01%	0.003%
16	3.355	717	720	722	rBV3	660	383	0.01%	0.002%
17	3.416	736	739	743	rVB4	628	394	0.01%	0.002%
18	3.432	743	744	746	rBV	548	238	0.00%	0.001%
19	3.506	765	767	768	rBV2	442	176	0.00%	0.001%
20	3.551	777	781	784	rBB5	520	267	0.00%	0.001%
21	3.590	791	793	797	rBV	513	273	0.00%	0.002%
22	3.648	807	811	814	rBV4	701	536	0.01%	0.003%
23	3.670	816	818	822	rBV3	560	372	0.01%	0.002%
24	3.725	831	835	838	rBV3	1164	739	0.01%	0.004%
25	3.812	858	862	863	rBV2	640	399	0.01%	0.002%
26	3.825	863	866	870	rVB3	542	421	0.01%	0.002%
27	3.902	870	890	909	rBV	2428164	5884501	100.00%	32.509%
28	4.342	1014	1027	1049	rBV	247256	630882	10.72%	3.485%
29	4.857	1184	1187	1188	rBV2	599	325	0.01%	0.002%
30	4.899	1195	1200	1201	rBV2	534	427	0.01%	0.002%
31	5.040	1228	1244	1288	rBV2	609544	1621972	27.56%	8.961%
32	5.355	1339	1342	1344	rBV4	1087	744	0.01%	0.004%
33	5.461	1372	1375	1377	rVB4	1009	533	0.01%	0.003%
34	5.481	1379	1381	1385	rVB3	1285	679	0.01%	0.004%
35	5.612	1410	1422	1461	rBV	370856	802367	13.64%	4.433%
36	5.908	1501	1514	1545	rBV	516877	1075883	18.28%	5.944%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027227.D
 Acq On : 05 Aug 2022 16:07
 Operator : SY/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.066	1552	1563	1592	rVB	357322	747196	12.70%	4.128%
38	6.342	1647	1649	1652	rBV3	1026	437	0.01%	0.002%
39	6.445	1679	1681	1682	rBV2	519	184	0.00%	0.001%
40	6.474	1688	1690	1693	rVB4	811	506	0.01%	0.003%
41	6.561	1714	1717	1719	rBV4	1466	1163	0.02%	0.006%
42	6.661	1746	1748	1752	rBV5	633	345	0.01%	0.002%
43	6.773	1781	1783	1786	rVB3	593	299	0.01%	0.002%
44	6.918	1826	1828	1832	rBV3	416	220	0.00%	0.001%
45	6.944	1834	1836	1838	rBV3	648	396	0.01%	0.002%
46	6.982	1838	1848	1872	rBV	166383	318612	5.41%	1.760%
47	7.313	1939	1951	1977	rBV	629571	1145005	19.46%	6.326%
48	7.619	2037	2046	2067	rBV	120075	217650	3.70%	1.202%
49	7.873	2123	2125	2131	rVB5	1236	971	0.02%	0.005%
50	7.898	2131	2133	2134	rBV3	494	207	0.00%	0.001%
51	7.979	2148	2158	2172	rBV6	10639	21294	0.36%	0.118%
52	8.088	2182	2192	2235	rBV	433239	868138	14.75%	4.796%
53	8.767	2401	2403	2405	rBV2	607	190	0.00%	0.001%
54	8.850	2417	2429	2459	rBV	614747	1012479	17.21%	5.593%
55	9.239	2548	2550	2551	rBV2	1140	371	0.01%	0.002%
56	9.358	2584	2587	2588	rBV3	581	252	0.00%	0.001%
57	9.410	2600	2603	2607	rBV4	567	424	0.01%	0.002%
58	9.455	2615	2617	2618	rBV2	610	223	0.00%	0.001%
59	9.570	2650	2653	2656	rBV4	733	610	0.01%	0.003%
60	9.609	2664	2665	2669	rBV3	483	321	0.01%	0.002%
61	9.628	2669	2671	2673	rBV2	475	180	0.00%	0.001%
62	9.654	2676	2679	2681	rBV3	565	336	0.01%	0.002%
63	9.734	2701	2704	2707	rBV2	624	546	0.01%	0.003%
64	10.101	2816	2818	2823	rVB4	909	621	0.01%	0.003%
65	10.159	2834	2836	2838	rBV	406	247	0.00%	0.001%
66	10.213	2841	2853	2876	rVV	512224	812235	13.80%	4.487%
67	10.422	2916	2918	2924	rBV4	663	662	0.01%	0.004%
68	10.500	2937	2942	2944	rBV5	632	660	0.01%	0.004%
69	10.529	2949	2951	2953	rVB3	903	384	0.01%	0.002%
70	10.541	2953	2955	2956	rBV	695	255	0.00%	0.001%
71	10.603	2972	2974	2976	rBV2	835	525	0.01%	0.003%
72	10.709	3004	3007	3011	rBV3	928	568	0.01%	0.003%
73	10.847	3048	3050	3056	rVB4	1266	983	0.02%	0.005%
74	10.905	3066	3068	3069	rBV2	740	313	0.01%	0.002%
75	10.940	3077	3079	3082	rBV3	410	269	0.00%	0.001%
76	10.953	3082	3083	3084	rBV	527	180	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027227.D
 Acq On : 05 Aug 2022 16:07
 Operator : SY/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.992	3091	3095	3097	rBV4	857	537	0.01%	0.003%
78	11.021	3103	3104	3106	rBV	403	205	0.00%	0.001%
79	11.056	3112	3115	3116	rBV2	657	289	0.00%	0.002%
80	11.146	3140	3143	3148	rBV4	449	444	0.01%	0.002%
81	11.246	3163	3174	3192	rBV	507231	795409	13.52%	4.394%
82	11.458	3238	3240	3244	rVB4	991	462	0.01%	0.003%
83	11.548	3266	3268	3273	rBV4	788	638	0.01%	0.004%
84	11.622	3279	3291	3309	rBV	610050	966475	16.42%	5.339%
85	11.905	3377	3379	3383	rBV4	1235	604	0.01%	0.003%
86	12.249	3482	3486	3488	rBV2	838	697	0.01%	0.004%
87	12.365	3520	3522	3525	rBV3	694	405	0.01%	0.002%
88	12.625	3601	3603	3605	rBV2	488	222	0.00%	0.001%
89	12.773	3647	3649	3651	rBV2	475	298	0.01%	0.002%
90	12.834	3665	3668	3671	rBV2	653	374	0.01%	0.002%
91	12.850	3671	3673	3676	rBV2	878	470	0.01%	0.003%
92	13.040	3730	3732	3734	rBV2	741	332	0.01%	0.002%
93	13.078	3742	3744	3748	rBV4	963	742	0.01%	0.004%
94	13.123	3756	3758	3762	rBV5	728	599	0.01%	0.003%
95	13.287	3806	3809	3812	rBV4	800	582	0.01%	0.003%
96	13.422	3849	3851	3853	rBV2	816	300	0.01%	0.002%
97	13.805	3968	3970	3974	rVB2	752	360	0.01%	0.002%
98	14.017	4033	4036	4038	rBV2	708	419	0.01%	0.002%
99	14.699	4246	4248	4251	rBV2	882	470	0.01%	0.003%
100	14.934	4318	4321	4325	rBV4	1037	750	0.01%	0.004%



Sum of corrected areas: 18101150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027227.D
Acq On : 05 Aug 2022 16:07
Operator : SY/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

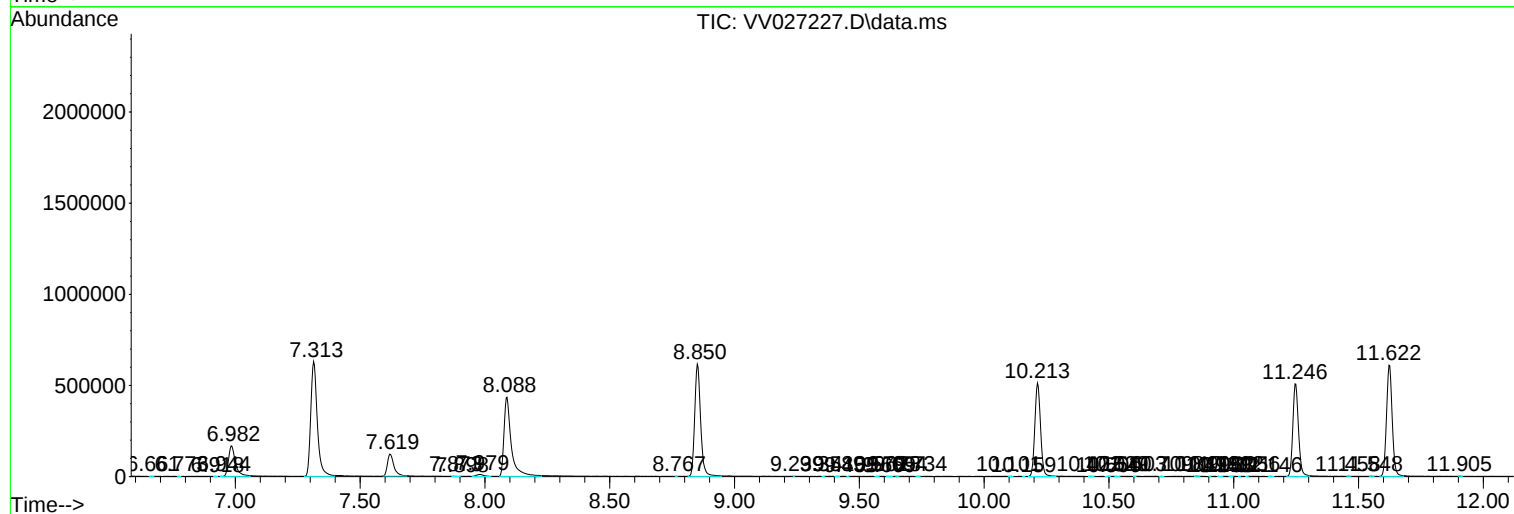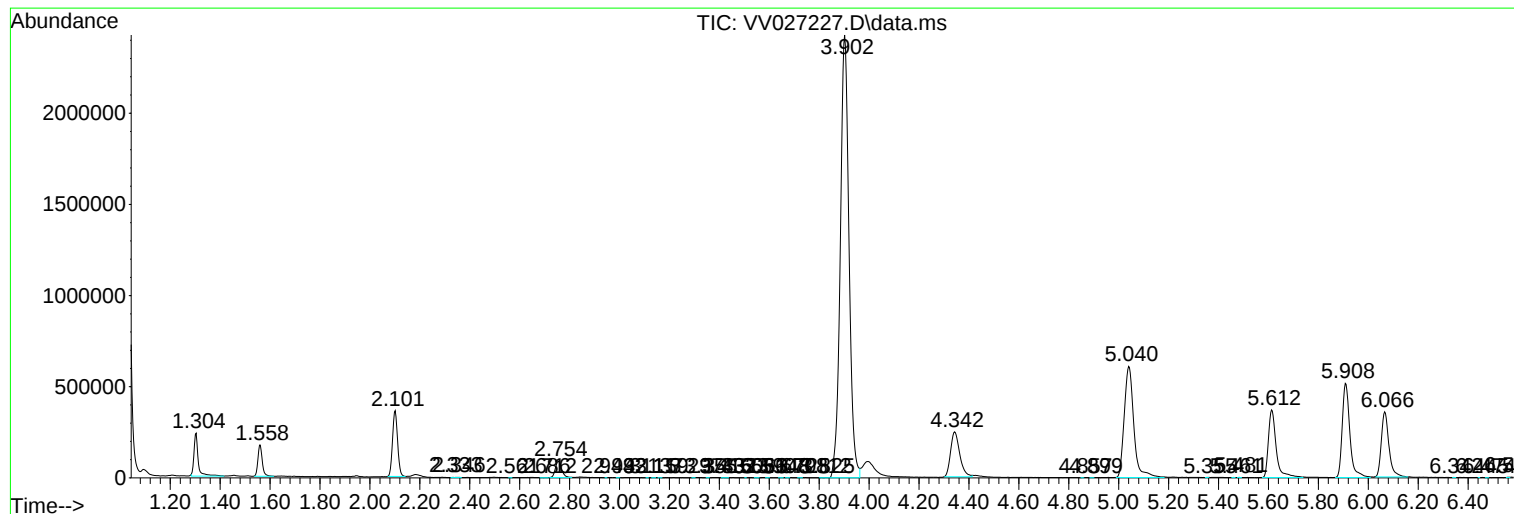

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027227.D
Acq On : 05 Aug 2022 16:07
Operator : SY/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027227.D
Acq On : 05 Aug 2022 16:07
Operator : SY/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc