

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027229.D
 Acq On : 05 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rBV2	594179	686235	6.67%	3.128%
2	1.558	154	161	174	rBV	175801	213009	2.07%	0.971%
3	2.102	321	330	344	rBV	365137	520257	5.06%	2.371%
4	2.687	510	512	518	rVB4	1068	765	0.01%	0.003%
5	2.712	518	520	522	rBV3	772	396	0.00%	0.002%
6	2.754	522	533	553	rBV	63935	122975	1.19%	0.560%
7	2.918	582	584	586	rBV3	956	441	0.00%	0.002%
8	2.931	586	588	590	rBV3	993	425	0.00%	0.002%
9	3.143	651	654	655	rBV2	736	326	0.00%	0.001%
10	3.368	721	724	727	rBV3	1133	841	0.01%	0.004%
11	3.404	731	735	737	rBV4	455	356	0.00%	0.002%
12	3.629	801	805	810	rVB5	507	535	0.01%	0.002%
13	3.757	829	845	851	rBV9	4574	9298	0.09%	0.042%
14	3.831	863	868	870	rBV3	1358	920	0.01%	0.004%
15	3.902	871	890	908	rBV	4324071	10291460	100.00%	46.904%
16	4.343	1013	1027	1064	rBV	252159	650915	6.32%	2.967%
17	4.835	1177	1180	1181	rBV2	836	506	0.00%	0.002%
18	4.928	1208	1209	1211	rVB2	924	326	0.00%	0.001%
19	4.941	1211	1213	1217	rBV3	651	505	0.00%	0.002%
20	5.040	1227	1244	1286	rBV2	617212	1646455	16.00%	7.504%
21	5.613	1409	1422	1459	rBV	365573	783934	7.62%	3.573%
22	5.912	1501	1515	1542	rBV5	78372	190241	1.85%	0.867%
23	6.066	1549	1563	1588	rBV	360577	765102	7.43%	3.487%
24	6.355	1651	1653	1658	rVB6	915	582	0.01%	0.003%
25	6.455	1680	1684	1689	rVB6	928	990	0.01%	0.005%
26	6.555	1713	1715	1717	rVB2	810	302	0.00%	0.001%
27	6.629	1736	1738	1741	rVB2	699	325	0.00%	0.001%
28	6.677	1751	1753	1757	rVB4	846	405	0.00%	0.002%
29	6.699	1757	1760	1764	rVB4	598	522	0.01%	0.002%
30	6.735	1769	1771	1774	rVB3	651	314	0.00%	0.001%
31	6.982	1837	1848	1872	rBV	166304	321341	3.12%	1.465%
32	7.314	1940	1951	1979	rBV	643262	1155448	11.23%	5.266%
33	7.619	2037	2046	2079	rVB	122164	222740	2.16%	1.015%
34	7.889	2128	2130	2133	rBV4	1156	481	0.00%	0.002%
35	7.982	2150	2159	2169	rBV7	5902	10384	0.10%	0.047%
36	8.047	2176	2179	2180	rBV2	706	292	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027229.D
 Acq On : 05 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	8.088	2182	2192	2220	rBV2	402974	813617	7.91%	3.708%
38	8.551	2334	2336	2339	rBV3	844	545	0.01%	0.002%
39	8.764	2399	2402	2404	rBV3	899	547	0.01%	0.002%
40	8.850	2416	2429	2459	rBV	578097	979557	9.52%	4.464%
41	9.185	2532	2533	2535	rBV2	597	293	0.00%	0.001%
42	9.278	2561	2562	2565	rBV3	797	264	0.00%	0.001%
43	9.371	2588	2591	2592	rBV2	789	319	0.00%	0.001%
44	9.481	2620	2625	2627	rBV4	738	680	0.01%	0.003%
45	9.519	2633	2637	2641	rVB6	973	858	0.01%	0.004%
46	9.542	2641	2644	2645	rBV2	832	398	0.00%	0.002%
47	9.571	2650	2653	2656	rBV5	822	418	0.00%	0.002%
48	9.606	2661	2664	2666	rBV3	516	312	0.00%	0.001%
49	9.641	2673	2675	2679	rBV3	578	329	0.00%	0.001%
50	9.722	2697	2700	2702	rBV3	619	328	0.00%	0.001%
51	9.773	2714	2716	2719	rVV3	599	326	0.00%	0.001%
52	9.789	2719	2721	2723	rVB2	708	267	0.00%	0.001%
53	9.953	2769	2772	2773	rBV2	558	316	0.00%	0.001%
54	9.973	2776	2778	2781	rBV3	541	331	0.00%	0.002%
55	10.014	2787	2791	2793	rBV3	640	422	0.00%	0.002%
56	10.140	2828	2830	2834	rBV5	459	380	0.00%	0.002%
57	10.214	2839	2853	2873	rBV	489985	772075	7.50%	3.519%
58	10.407	2910	2913	2914	rBV2	677	439	0.00%	0.002%
59	10.500	2940	2942	2943	rBV	754	259	0.00%	0.001%
60	10.535	2950	2953	2954	rBV3	515	282	0.00%	0.001%
61	10.645	2984	2987	2990	rBV4	742	531	0.01%	0.002%
62	10.674	2990	2996	2997	rVV4	592	459	0.00%	0.002%
63	10.696	3001	3003	3006	rBV	561	392	0.00%	0.002%
64	10.722	3009	3011	3013	rBV	472	309	0.00%	0.001%
65	10.776	3025	3028	3031	rBV4	789	553	0.01%	0.003%
66	10.793	3031	3033	3036	rVB3	654	355	0.00%	0.002%
67	10.895	3063	3065	3070	rVB5	737	566	0.01%	0.003%
68	10.924	3070	3074	3076	rBV3	734	675	0.01%	0.003%
69	11.047	3110	3112	3116	rBV2	547	490	0.00%	0.002%
70	11.066	3116	3118	3119	rBV	630	309	0.00%	0.001%
71	11.156	3143	3146	3148	rBV3	657	383	0.00%	0.002%
72	11.175	3148	3152	3154	rBV	503	317	0.00%	0.001%
73	11.249	3163	3175	3195	rBV	496201	772921	7.51%	3.523%
74	11.477	3243	3246	3250	rVB6	942	687	0.01%	0.003%
75	11.497	3250	3252	3256	rVB3	504	282	0.00%	0.001%
76	11.548	3256	3268	3272	rBV9	1764	3538	0.03%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027229.D
 Acq On : 05 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.622	3280	3291	3309	rBV	612486	972824	9.45%	4.434%
78	12.114	3442	3444	3447	rBV4	555	402	0.00%	0.002%
79	12.300	3498	3502	3506	rBV5	707	697	0.01%	0.003%
80	12.355	3517	3519	3521	rBV2	793	504	0.00%	0.002%
81	12.439	3544	3545	3550	rBV3	821	622	0.01%	0.003%
82	12.484	3557	3559	3562	rVB4	930	438	0.00%	0.002%
83	12.616	3598	3600	3604	rVB4	771	407	0.00%	0.002%
84	12.638	3604	3607	3609	rBV3	557	404	0.00%	0.002%
85	12.863	3675	3677	3678	rBV2	610	290	0.00%	0.001%
86	12.985	3712	3715	3716	rBV2	703	352	0.00%	0.002%
87	13.005	3719	3721	3724	rVB2	689	382	0.00%	0.002%
88	13.342	3822	3826	3828	rBV3	774	477	0.00%	0.002%
89	13.464	3862	3864	3871	rVB4	1111	980	0.01%	0.004%
90	13.876	3990	3992	3995	rBV3	919	522	0.01%	0.002%
91	13.989	4023	4027	4029	rBV3	1028	748	0.01%	0.003%
92	14.050	4044	4046	4053	rVB4	756	660	0.01%	0.003%
93	14.169	4080	4083	4086	rBV3	608	392	0.00%	0.002%
94	14.243	4103	4106	4109	rBV4	845	675	0.01%	0.003%
95	14.278	4115	4117	4119	rBV3	583	292	0.00%	0.001%
96	14.744	4260	4262	4266	rBV3	744	735	0.01%	0.003%
97	14.847	4292	4294	4298	rVB2	1154	565	0.01%	0.003%
98	14.863	4298	4299	4304	rBV3	708	335	0.00%	0.002%
99	15.024	4346	4349	4350	rBV	817	466	0.00%	0.002%
100	15.095	4370	4371	4377	rBV6	1169	924	0.01%	0.004%




Sum of corrected areas: 21941771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027229.D
Acq On : 05 Aug 2022 16:57
Operator : SY/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

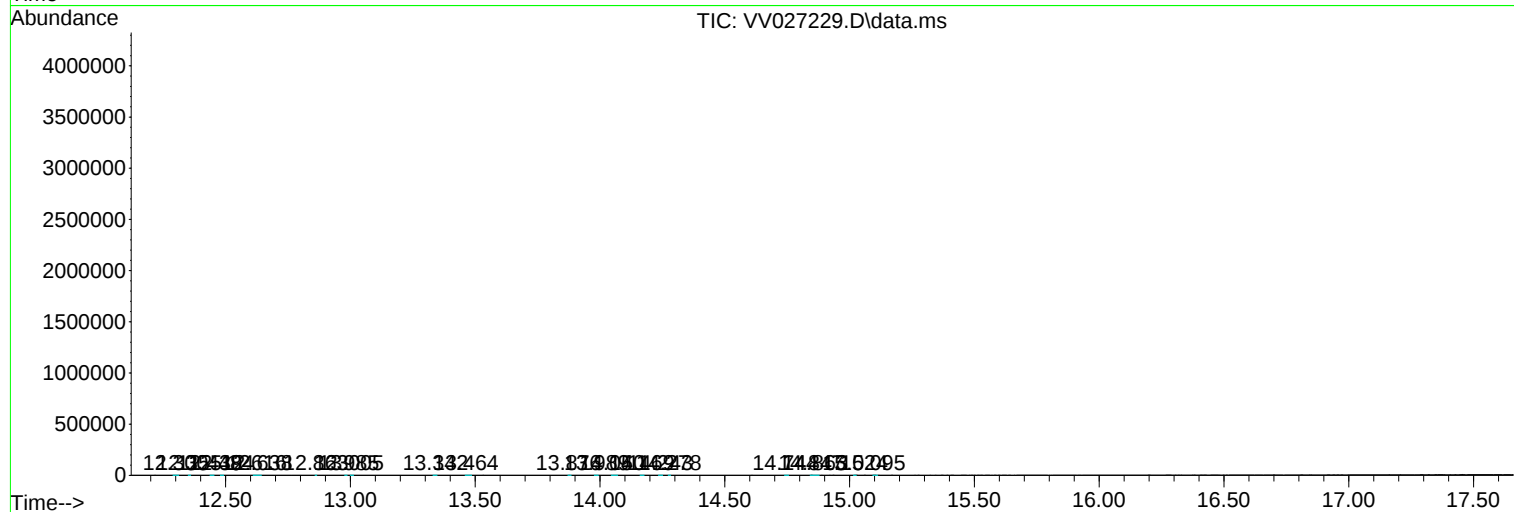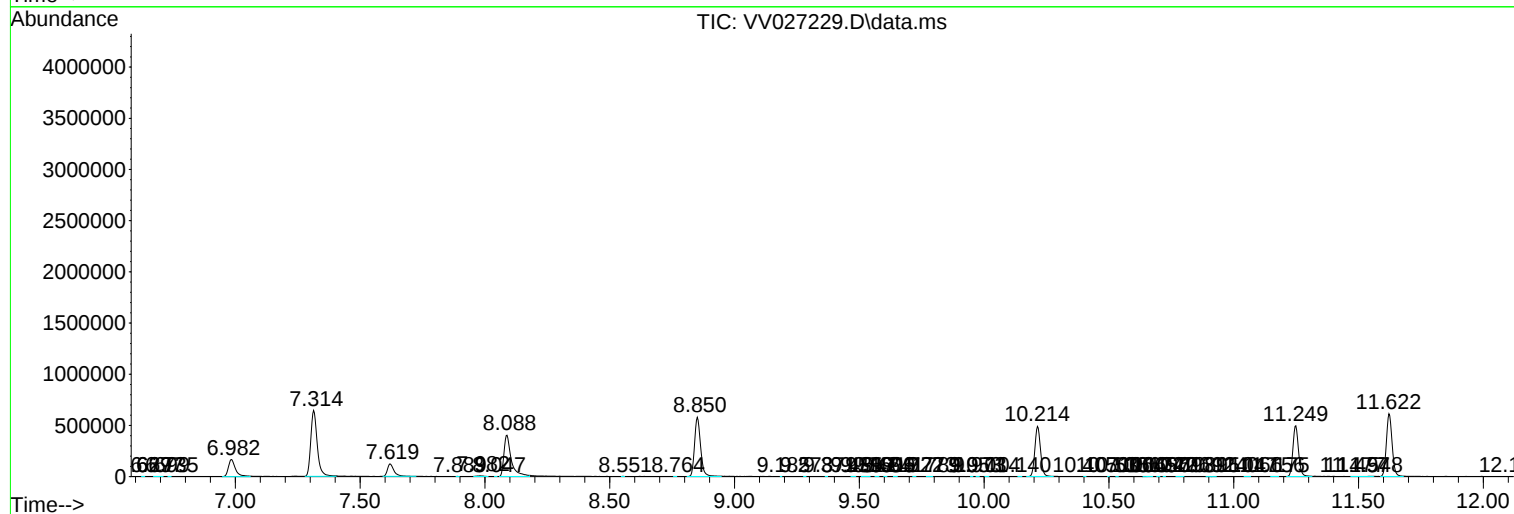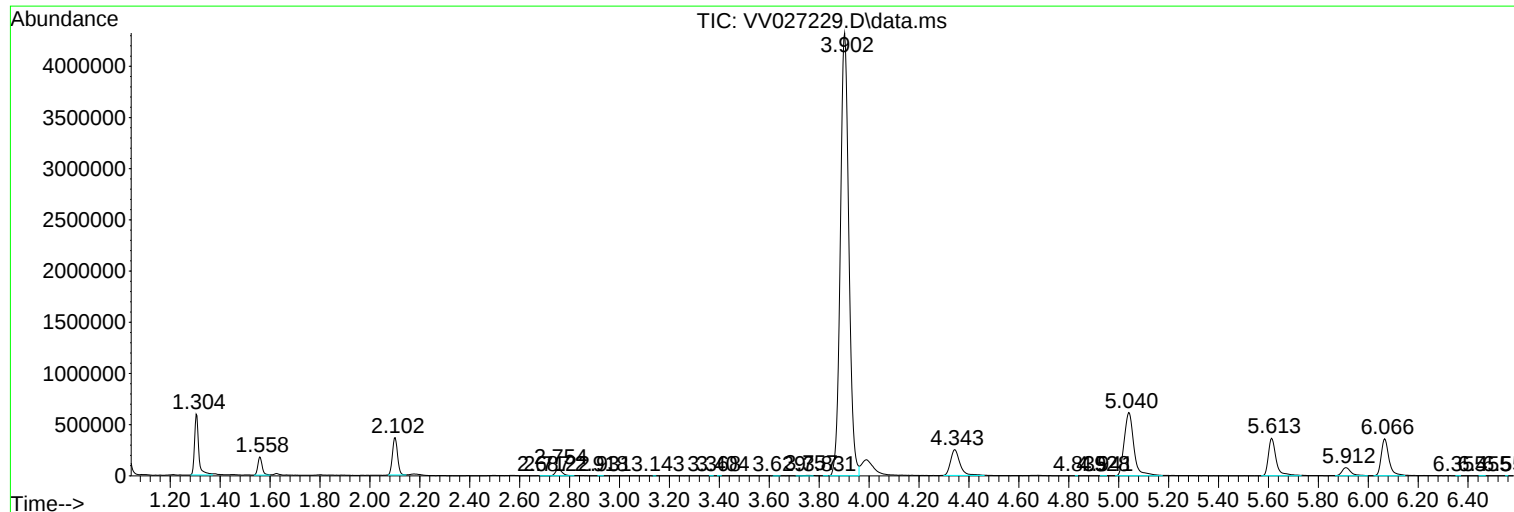

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027229.D
Acq On : 05 Aug 2022 16:57
Operator : SY/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027229.D
Acq On : 05 Aug 2022 16:57
Operator : SY/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------