

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027230.D
 Acq On : 05 Aug 2022 17:22
 Operator : SY/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV2	415535	476772	10.64%	2.153%
2	1.561	155	162	177	rVB2	170871	230555	5.14%	1.041%
3	2.101	321	330	345	rBV2	373834	539594	12.04%	2.437%
4	2.616	487	490	495	rBV4	794	752	0.02%	0.003%
5	2.712	517	520	523	rBV	506	361	0.01%	0.002%
6	2.757	523	534	552	rBV2	36195	70985	1.58%	0.321%
7	2.969	598	600	601	rBV2	741	295	0.01%	0.001%
8	3.121	643	647	648	rBV2	1107	547	0.01%	0.002%
9	3.153	655	657	658	rBV	528	175	0.00%	0.001%
10	3.185	663	667	670	rBV	921	602	0.01%	0.003%
11	3.207	672	674	676	rVB	757	216	0.00%	0.001%
12	3.233	680	682	683	rBV2	554	270	0.01%	0.001%
13	3.262	688	691	693	rBV2	743	478	0.01%	0.002%
14	3.297	700	702	703	rBV	375	115	0.00%	0.001%
15	3.320	707	709	711	rVB2	381	160	0.00%	0.001%
16	3.336	711	714	717	rBV2	444	377	0.01%	0.002%
17	3.358	717	721	723	rBV2	519	324	0.01%	0.001%
18	3.391	729	731	732	rBV2	229	96	0.00%	0.000%
19	3.465	749	754	757	rBV2	818	703	0.02%	0.003%
20	3.494	760	763	765	rBV3	494	262	0.01%	0.001%
21	3.510	765	768	769	rBV2	487	207	0.00%	0.001%
22	3.522	769	772	776	rVB3	869	555	0.01%	0.003%
23	3.577	787	789	790	rBV	402	122	0.00%	0.001%
24	3.625	799	804	805	rBV4	558	389	0.01%	0.002%
25	3.645	809	810	812	rBV2	378	140	0.00%	0.001%
26	3.661	814	815	817	rBV	378	139	0.00%	0.001%
27	3.677	817	820	822	rBV4	696	431	0.01%	0.002%
28	3.719	830	833	834	rBV2	526	304	0.01%	0.001%
29	3.812	858	862	863	rBV3	654	359	0.01%	0.002%
30	3.902	871	890	910	rBV2	1446656	3672096	81.94%	16.584%
31	4.342	1014	1027	1061	rBV	252285	652316	14.56%	2.946%
32	4.487	1069	1072	1081	rVB	14702	9891	0.22%	0.045%
33	4.911	1202	1204	1205	rBV2	759	311	0.01%	0.001%
34	4.953	1213	1217	1218	rBV3	616	352	0.01%	0.002%
35	4.976	1219	1224	1227	rBV4	975	778	0.02%	0.004%
36	5.040	1227	1244	1289	rBV2	616952	1658186	37.00%	7.489%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027230.D
 Acq On : 05 Aug 2022 17:22
 Operator : SY/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	5.506	1387	1389	1390	rBV2	662	229	0.01%	0.001%
38	5.612	1411	1422	1457	rBV	372766	794545	17.73%	3.588%
39	5.908	1500	1514	1547	rBV	1235044	2520879	56.25%	11.385%
40	6.066	1552	1563	1594	rVB	367155	775913	17.31%	3.504%
41	6.709	1761	1763	1764	rVB2	687	156	0.00%	0.001%
42	6.718	1764	1766	1770	rVB3	661	348	0.01%	0.002%
43	6.825	1798	1799	1801	rBV3	636	268	0.01%	0.001%
44	6.889	1817	1819	1823	rBV3	932	703	0.02%	0.003%
45	6.908	1823	1825	1827	rBV2	495	261	0.01%	0.001%
46	6.934	1830	1833	1835	rBV4	570	357	0.01%	0.002%
47	6.985	1838	1849	1871	rBV	168579	320916	7.16%	1.449%
48	7.313	1940	1951	1975	rBV	649474	1171495	26.14%	5.291%
49	7.619	2037	2046	2067	rBV	122943	223704	4.99%	1.010%
50	7.972	2142	2156	2182	rBV	2627899	4481214	100.00%	20.239%
51	8.088	2183	2192	2231	rVB	466792	900896	20.10%	4.069%
52	8.850	2418	2429	2450	rBV	607587	1004209	22.41%	4.535%
53	9.111	2507	2510	2515	rBV4	1271	1269	0.03%	0.006%
54	9.178	2529	2531	2534	rBV4	722	353	0.01%	0.002%
55	9.342	2577	2582	2584	rBV4	1063	628	0.01%	0.003%
56	9.355	2584	2586	2588	rBV	671	359	0.01%	0.002%
57	9.394	2596	2598	2602	rVB2	1101	575	0.01%	0.003%
58	9.493	2628	2629	2631	rBV2	823	373	0.01%	0.002%
59	9.660	2679	2681	2682	rBV2	693	334	0.01%	0.002%
60	9.680	2685	2687	2688	rBV2	685	225	0.01%	0.001%
61	9.722	2698	2700	2701	rVB	457	105	0.00%	0.000%
62	9.767	2713	2714	2715	rBV	475	122	0.00%	0.001%
63	9.876	2746	2748	2751	rBV3	828	329	0.01%	0.001%
64	9.940	2764	2768	2771	rBV3	1049	767	0.02%	0.003%
65	9.992	2782	2784	2787	rVB2	677	333	0.01%	0.002%
66	10.059	2802	2805	2809	rBV4	597	529	0.01%	0.002%
67	10.169	2837	2839	2841	rVB2	626	217	0.00%	0.001%
68	10.214	2841	2853	2881	rBV	511000	813018	18.14%	3.672%
69	10.361	2896	2899	2903	rBV3	827	704	0.02%	0.003%
70	10.464	2928	2931	2933	rBV4	620	376	0.01%	0.002%
71	10.818	3037	3041	3044	rBV3	542	525	0.01%	0.002%
72	10.972	3085	3089	3093	rBB2	960	784	0.02%	0.004%
73	11.024	3101	3105	3106	rBV2	378	257	0.01%	0.001%
74	11.056	3112	3115	3116	rBV2	536	258	0.01%	0.001%
75	11.191	3153	3157	3159	rBV4	1120	944	0.02%	0.004%
76	11.249	3162	3175	3199	rBV	507621	804795	17.96%	3.635%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027230.D
 Acq On : 05 Aug 2022 17:22
 Operator : SY/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

77	11.519	3256	3259	3262	rBV3	1162	790	0.02%	0.004%
78	11.625	3280	3292	3311	rBV	615675	990953	22.11%	4.475%
79	12.442	3542	3546	3547	rBV3	830	591	0.01%	0.003%
80	12.461	3550	3552	3553	rBV2	629	287	0.01%	0.001%
81	12.609	3595	3598	3600	rBV3	691	431	0.01%	0.002%
82	12.815	3660	3662	3665	rBV3	707	546	0.01%	0.002%
83	12.908	3689	3691	3693	rBV3	958	458	0.01%	0.002%
84	12.937	3698	3700	3706	rVB4	834	489	0.01%	0.002%
85	12.992	3716	3717	3720	rBV2	567	273	0.01%	0.001%
86	13.438	3854	3856	3859	rVB3	846	469	0.01%	0.002%
87	13.956	4013	4017	4019	rBV3	963	696	0.02%	0.003%
88	14.319	4128	4130	4131	rBV	628	253	0.01%	0.001%
89	14.599	4215	4217	4219	rBV	657	402	0.01%	0.002%
90	15.017	4345	4347	4349	rVB3	1136	400	0.01%	0.002%
91	15.107	4374	4375	4378	rBV3	1023	484	0.01%	0.002%


Sum of corrected areas: 22142009

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027230.D
Acq On : 05 Aug 2022 17:22
Operator : SY/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

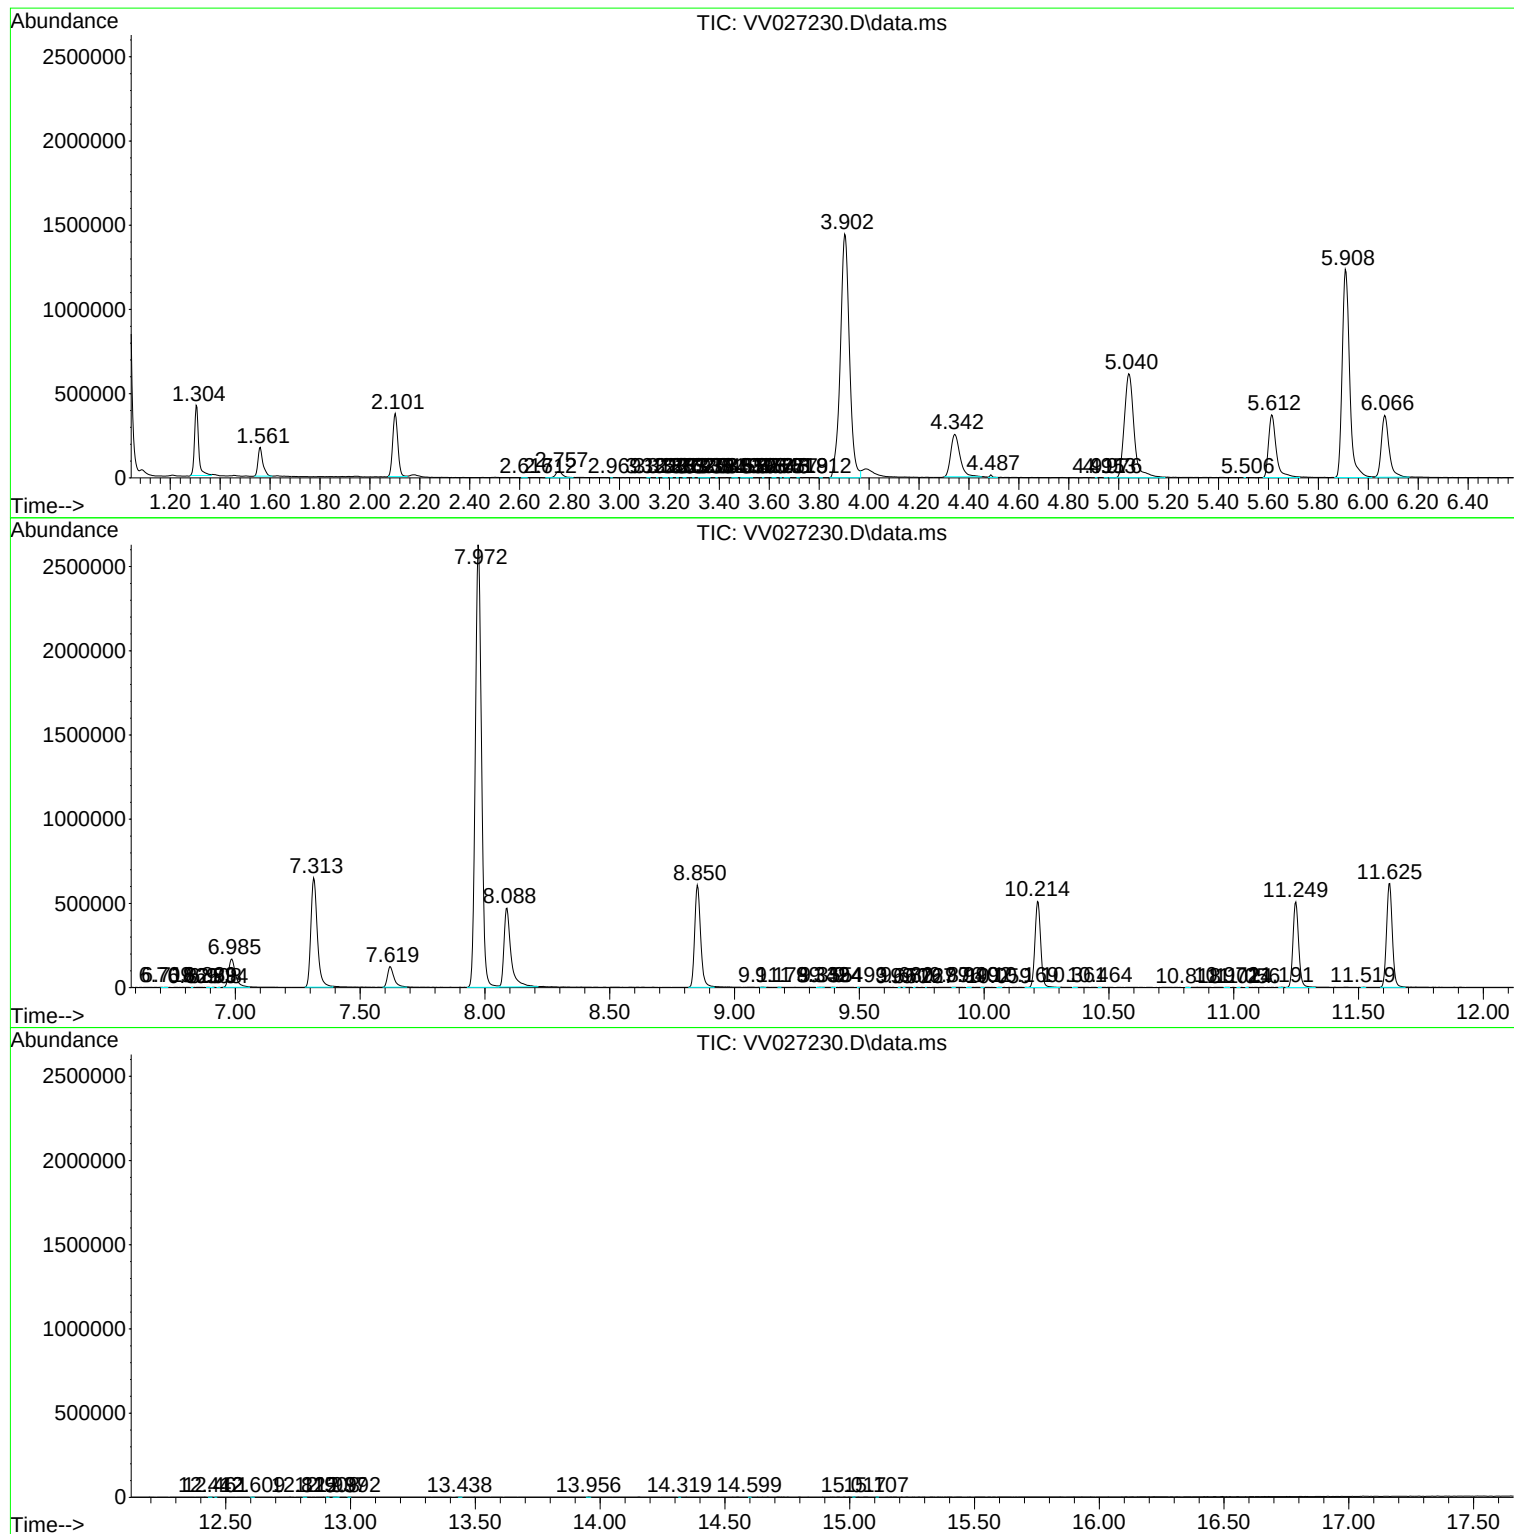

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027230.D
Acq On : 05 Aug 2022 17:22
Operator : SY/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027230.D
Acq On : 05 Aug 2022 17:22
Operator : SY/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc