

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027231.D
 Acq On : 05 Aug 2022 17:47
 Operator : SY/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB2	313680	357784	15.03%	2.514%
2	1.558	154	161	178	rVB	169244	224250	9.42%	1.576%
3	2.098	320	329	342	rBV	357396	511669	21.50%	3.595%
4	2.346	404	406	408	rBV2	925	421	0.02%	0.003%
5	2.722	520	523	524	rBV	588	375	0.02%	0.003%
6	2.757	524	534	549	rVV2	24994	47989	2.02%	0.337%
7	3.027	616	618	621	rBV3	817	442	0.02%	0.003%
8	3.072	631	632	634	rBV2	847	315	0.01%	0.002%
9	3.114	643	645	652	rVB4	661	606	0.03%	0.004%
10	3.143	652	654	659	rBV3	616	492	0.02%	0.003%
11	3.175	659	664	667	rBV3	770	668	0.03%	0.005%
12	3.198	667	671	675	rVB4	745	606	0.03%	0.004%
13	3.259	688	690	693	rVB2	848	456	0.02%	0.003%
14	3.281	693	697	699	rVB2	815	457	0.02%	0.003%
15	3.304	699	704	707	rBV4	745	589	0.02%	0.004%
16	3.336	711	714	718	rBV4	639	568	0.02%	0.004%
17	3.497	760	764	767	rVB5	809	695	0.03%	0.005%
18	3.674	816	819	823	rVB4	757	450	0.02%	0.003%
19	3.699	823	827	831	rBV4	550	580	0.02%	0.004%
20	3.741	837	840	842	rBV3	575	468	0.02%	0.003%
21	3.902	867	890	911	rBV2	887858	2379827	100.00%	16.723%
22	4.343	1013	1027	1048	rBV	252193	643828	27.05%	4.524%
23	4.638	1117	1119	1120	rBV	846	300	0.01%	0.002%
24	4.735	1146	1149	1152	rBV4	951	569	0.02%	0.004%
25	4.767	1157	1159	1161	rBV2	674	321	0.01%	0.002%
26	4.857	1185	1187	1190	rVB3	559	302	0.01%	0.002%
27	4.873	1190	1192	1194	rBV3	722	380	0.02%	0.003%
28	4.947	1209	1215	1219	rBV5	763	853	0.04%	0.006%
29	5.040	1226	1244	1288	rBV2	610594	1654931	69.54%	11.629%
30	5.494	1383	1385	1388	rVB3	1210	547	0.02%	0.004%
31	5.526	1392	1395	1398	rBV5	964	635	0.03%	0.004%
32	5.613	1410	1422	1440	rBV	365883	751727	31.59%	5.282%
33	5.912	1501	1515	1542	rBV2	227847	489468	20.57%	3.439%
34	6.066	1551	1563	1592	rBV	361830	753910	31.68%	5.298%
35	6.413	1669	1671	1674	rVB3	819	380	0.02%	0.003%
36	6.481	1688	1692	1693	rBV4	646	455	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027231.D
 Acq On : 05 Aug 2022 17:47
 Operator : SY/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1706	rVB2	885	493	0.02%	0.003%
38	6.539	1706	1710	1712	rBV4	1060	915	0.04%	0.006%
39	6.641	1739	1742	1743	rBV2	658	314	0.01%	0.002%
40	6.754	1776	1777	1779	rVB	1329	364	0.02%	0.003%
41	6.770	1779	1782	1784	rVB2	668	422	0.02%	0.003%
42	6.789	1784	1788	1790	rBV4	834	606	0.03%	0.004%
43	6.825	1796	1799	1801	rVB3	535	305	0.01%	0.002%
44	6.844	1803	1805	1808	rVV3	727	356	0.01%	0.003%
45	6.892	1819	1820	1822	rBV2	605	319	0.01%	0.002%
46	6.921	1827	1829	1831	rBV2	1008	370	0.02%	0.003%
47	6.986	1838	1849	1883	rBV	163176	322033	13.53%	2.263%
48	7.313	1939	1951	1975	rBV	635844	1157002	48.62%	8.130%
49	7.619	2036	2046	2070	rBV	120815	222432	9.35%	1.563%
50	7.924	2139	2141	2142	rBV2	901	371	0.02%	0.003%
51	7.976	2145	2157	2179	rBV	149833	265684	11.16%	1.867%
52	8.088	2182	2192	2222	rBV2	432178	845114	35.51%	5.939%
53	8.490	2315	2317	2321	rBV4	897	646	0.03%	0.005%
54	8.760	2399	2401	2403	rBV2	769	355	0.01%	0.002%
55	8.850	2418	2429	2459	rBV	590145	999170	41.98%	7.021%
56	9.278	2558	2562	2566	rBV3	906	631	0.03%	0.004%
57	9.378	2589	2593	2599	rVB4	862	1008	0.04%	0.007%
58	9.551	2642	2647	2652	rBV7	1824	2430	0.10%	0.017%
59	9.619	2665	2668	2673	rVB5	626	435	0.02%	0.003%
60	9.706	2693	2695	2698	rVB2	977	514	0.02%	0.004%
61	9.757	2706	2711	2714	rBV5	1060	825	0.03%	0.006%
62	9.825	2729	2732	2734	rBV2	744	530	0.02%	0.004%
63	9.857	2740	2742	2744	rVB3	902	441	0.02%	0.003%
64	9.902	2753	2756	2761	rBV3	625	551	0.02%	0.004%
65	9.940	2765	2768	2770	rBV2	706	357	0.02%	0.003%
66	10.149	2830	2833	2836	rBV3	529	384	0.02%	0.003%
67	10.214	2841	2853	2876	rBV	515401	809883	34.03%	5.691%
68	10.423	2916	2918	2922	rVB3	1003	573	0.02%	0.004%
69	10.448	2922	2926	2928	rBV5	846	720	0.03%	0.005%
70	10.529	2949	2951	2960	rVB6	1075	1329	0.06%	0.009%
71	10.577	2960	2966	2968	rBV5	1127	878	0.04%	0.006%
72	10.622	2979	2980	2983	rBV2	525	304	0.01%	0.002%
73	10.931	3072	3076	3077	rBV3	710	348	0.01%	0.002%
74	10.947	3079	3081	3086	rVB3	732	511	0.02%	0.004%
75	10.976	3086	3090	3091	rBV	605	416	0.02%	0.003%
76	11.008	3098	3100	3103	rBV	645	393	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027231.D
 Acq On : 05 Aug 2022 17:47
 Operator : SY/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.111	3130	3132	3137	rBV3	462	452	0.02%	0.003%
78	11.146	3141	3143	3145	rBV2	652	378	0.02%	0.003%
79	11.249	3164	3175	3192	rBV	498066	782483	32.88%	5.498%
80	11.622	3280	3291	3311	rBV	614070	966131	40.60%	6.789%
81	12.021	3411	3415	3419	rBV5	1014	1031	0.04%	0.007%
82	12.181	3463	3465	3469	rBV4	867	547	0.02%	0.004%
83	12.204	3469	3472	3476	rBV4	954	728	0.03%	0.005%
84	12.259	3487	3489	3493	rVB5	1044	612	0.03%	0.004%
85	12.326	3508	3510	3514	rVB2	838	498	0.02%	0.003%
86	12.352	3514	3518	3521	rBV3	600	570	0.02%	0.004%
87	12.532	3571	3574	3576	rBV2	588	353	0.01%	0.002%
88	12.570	3583	3586	3592	rVB5	1064	968	0.04%	0.007%
89	12.886	3679	3684	3689	rBV6	991	1073	0.05%	0.008%
90	12.937	3696	3700	3707	rVB5	815	779	0.03%	0.005%
91	13.152	3763	3767	3768	rBV3	662	429	0.02%	0.003%
92	13.262	3797	3801	3805	rBV4	857	801	0.03%	0.006%
93	13.429	3848	3853	3856	rBV5	659	606	0.03%	0.004%
94	13.596	3903	3905	3909	rBB3	554	350	0.01%	0.002%
95	13.757	3952	3955	3959	rBV3	687	526	0.02%	0.004%
96	13.779	3959	3962	3966	rVV6	659	607	0.03%	0.004%
97	13.857	3984	3986	3988	rBV3	464	324	0.01%	0.002%
98	13.924	4004	4007	4012	rBV5	929	926	0.04%	0.007%
99	14.387	4149	4151	4154	rBV3	772	394	0.02%	0.003%
100	14.722	4253	4255	4257	rBV2	620	387	0.02%	0.003%




Sum of corrected areas: 14230998

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027231.D
Acq On : 05 Aug 2022 17:47
Operator : SY/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

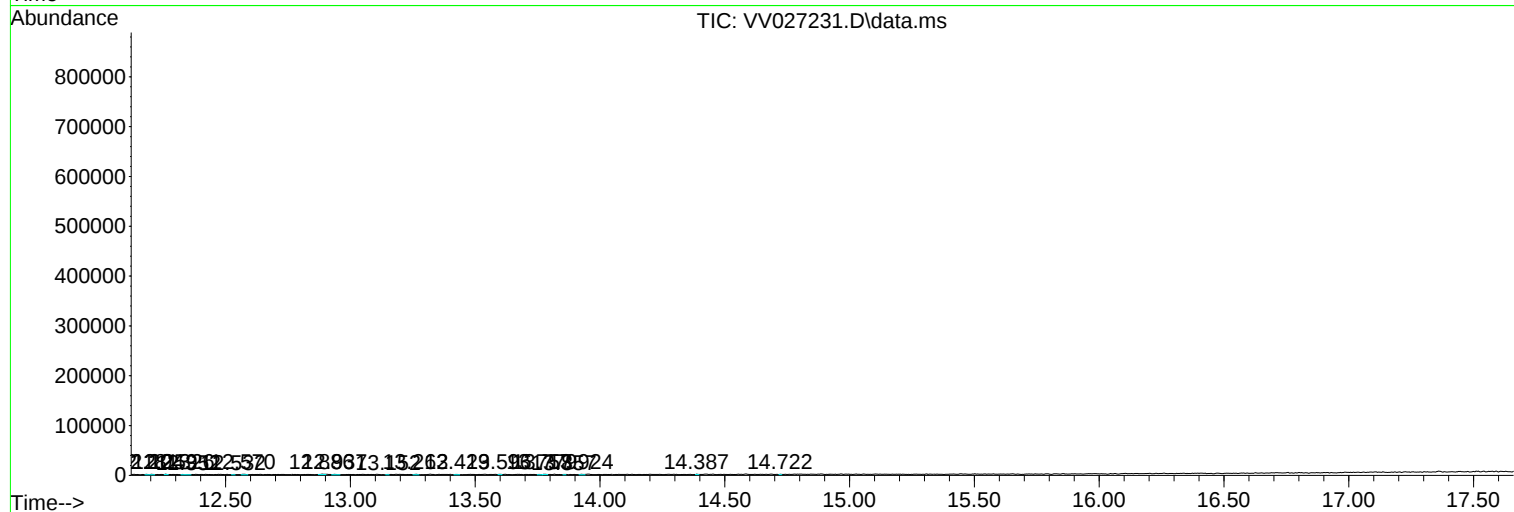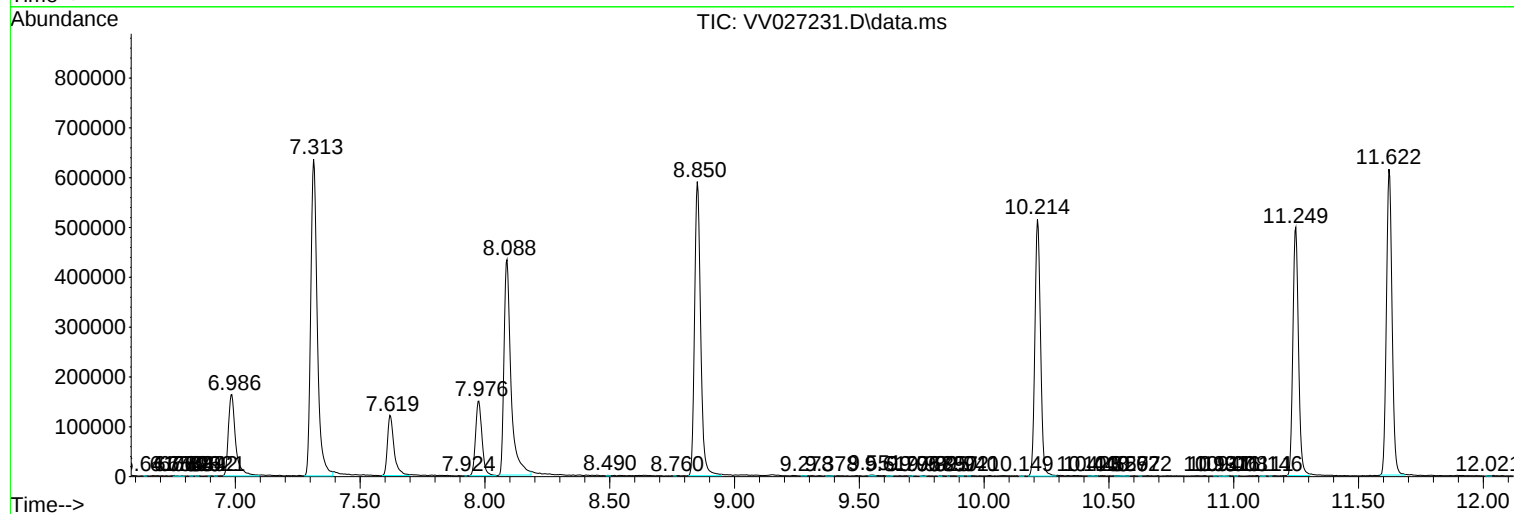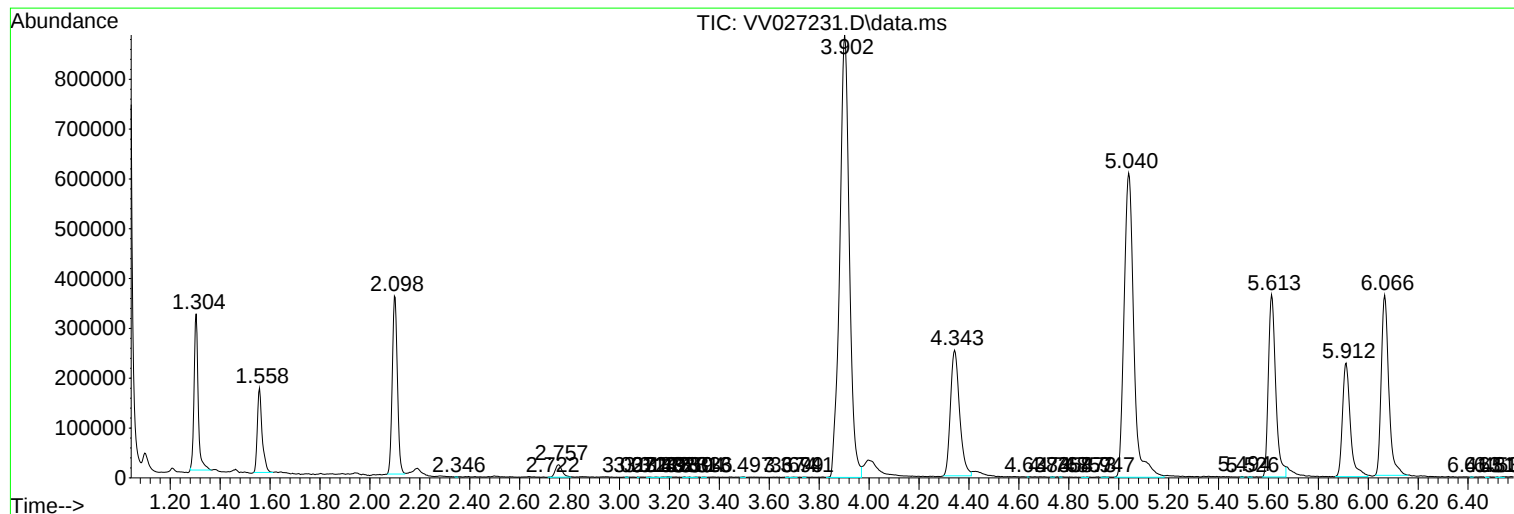

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027231.D
Acq On : 05 Aug 2022 17:47
Operator : SY/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027231.D
Acq On : 05 Aug 2022 17:47
Operator : SY/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc