

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027233.D
 Acq On : 05 Aug 2022 18:37
 Operator : SY/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB2	276264	296958	18.04%	2.397%
2	1.558	155	161	178	rVB	173774	205038	12.45%	1.655%
3	2.098	320	329	343	rBV	350129	497868	30.24%	4.019%
4	2.462	440	442	445	rBV2	720	351	0.02%	0.003%
5	2.494	447	452	453	rBV3	2495	1900	0.12%	0.015%
6	2.545	467	468	470	rBV	625	339	0.02%	0.003%
7	2.619	489	491	492	rBV	834	297	0.02%	0.002%
8	2.754	523	533	548	rBV2	63813	117532	7.14%	0.949%
9	2.915	581	583	586	rVB2	760	360	0.02%	0.003%
10	2.931	586	588	590	rBV2	609	292	0.02%	0.002%
11	2.960	594	597	599	rBV3	968	554	0.03%	0.004%
12	3.050	622	625	627	rBV2	719	363	0.02%	0.003%
13	3.162	658	660	663	rVB2	546	269	0.02%	0.002%
14	3.314	703	707	710	rVB3	710	489	0.03%	0.004%
15	3.336	710	714	719	rBV4	968	1077	0.07%	0.009%
16	3.381	723	728	731	rBV5	798	622	0.04%	0.005%
17	3.478	754	758	763	rVB3	579	527	0.03%	0.004%
18	3.523	769	772	774	rVV3	431	259	0.02%	0.002%
19	3.539	776	777	781	rBV2	648	288	0.02%	0.002%
20	3.635	799	807	809	rBV4	908	1166	0.07%	0.009%
21	3.670	817	818	821	rVB3	521	295	0.02%	0.002%
22	3.719	830	833	836	rBV3	479	333	0.02%	0.003%
23	3.802	857	859	863	rBV3	803	690	0.04%	0.006%
24	3.899	870	889	913	rBV2	253876	884310	53.72%	7.139%
25	4.342	1013	1027	1049	rBV	251109	640186	38.89%	5.168%
26	4.622	1112	1114	1118	rBV3	978	763	0.05%	0.006%
27	4.931	1206	1210	1211	rBV3	504	309	0.02%	0.002%
28	4.941	1211	1213	1215	rVV2	535	250	0.02%	0.002%
29	5.040	1226	1244	1295	rVV2	609888	1646247	100.00%	13.289%
30	5.613	1408	1422	1455	rBV	412465	885409	53.78%	7.147%
31	5.905	1502	1513	1532	rBV7	12697	32613	1.98%	0.263%
32	6.011	1542	1546	1547	rBV3	843	636	0.04%	0.005%
33	6.066	1550	1563	1590	rBV	356353	768475	46.68%	6.203%
34	6.326	1642	1644	1646	rBV2	936	605	0.04%	0.005%
35	6.413	1667	1671	1674	rBV4	1144	773	0.05%	0.006%
36	6.686	1753	1756	1757	rBV2	483	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027233.D
 Acq On : 05 Aug 2022 18:37
 Operator : SY/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.709	1760	1763	1766	rBV4	772	528	0.03%	0.004%
38	6.748	1773	1775	1777	rVB3	675	299	0.02%	0.002%
39	6.760	1777	1779	1781	rBV2	743	326	0.02%	0.003%
40	6.821	1795	1798	1801	rBV2	369	275	0.02%	0.002%
41	6.847	1801	1806	1809	rVV6	507	540	0.03%	0.004%
42	6.985	1837	1849	1875	rBV	163032	321025	19.50%	2.591%
43	7.313	1939	1951	1977	rBV	631545	1146010	69.61%	9.251%
44	7.619	2036	2046	2069	rBV	123027	225660	13.71%	1.822%
45	7.953	2148	2150	2152	rBV3	753	405	0.02%	0.003%
46	7.982	2152	2159	2166	rVV9	2944	4204	0.26%	0.034%
47	8.088	2182	2192	2229	rBV	436081	869600	52.82%	7.020%
48	8.587	2345	2347	2352	rBV5	1192	1102	0.07%	0.009%
49	8.751	2394	2398	2400	rBV4	879	591	0.04%	0.005%
50	8.850	2416	2429	2456	rBV	677203	1115611	67.77%	9.006%
51	9.207	2538	2540	2546	rBV7	1358	1148	0.07%	0.009%
52	9.233	2546	2548	2551	rVB3	947	458	0.03%	0.004%
53	9.252	2551	2554	2555	rBV3	710	420	0.03%	0.003%
54	9.339	2579	2581	2583	rVB2	883	413	0.03%	0.003%
55	9.362	2586	2588	2590	rBV2	757	282	0.02%	0.002%
56	9.471	2619	2622	2623	rBV3	807	392	0.02%	0.003%
57	9.661	2678	2681	2683	rBV3	551	377	0.02%	0.003%
58	9.718	2696	2699	2700	rBV2	944	497	0.03%	0.004%
59	9.802	2723	2725	2729	rBV4	624	330	0.02%	0.003%
60	9.828	2729	2733	2734	rBV	842	577	0.04%	0.005%
61	9.870	2742	2746	2750	rVB4	625	506	0.03%	0.004%
62	9.927	2761	2764	2766	rBV3	696	471	0.03%	0.004%
63	9.969	2774	2777	2780	rBV5	669	430	0.03%	0.003%
64	10.001	2782	2787	2791	rBV3	719	764	0.05%	0.006%
65	10.130	2821	2827	2831	rBV4	857	1002	0.06%	0.008%
66	10.169	2837	2839	2842	rBV3	681	454	0.03%	0.004%
67	10.214	2842	2853	2871	rVV	517312	817590	49.66%	6.600%
68	10.368	2899	2901	2903	rBV4	878	524	0.03%	0.004%
69	10.394	2907	2909	2911	rVB3	941	408	0.02%	0.003%
70	10.513	2944	2946	2948	rBV	772	342	0.02%	0.003%
71	10.683	2995	2999	3002	rBV4	752	612	0.04%	0.005%
72	10.718	3006	3010	3011	rBV2	621	380	0.02%	0.003%
73	10.815	3038	3040	3044	rVB4	939	442	0.03%	0.004%
74	10.918	3070	3072	3073	rBV	781	379	0.02%	0.003%
75	10.950	3080	3082	3085	rBV3	738	426	0.03%	0.003%
76	11.120	3133	3135	3139	rVB3	574	315	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027233.D
 Acq On : 05 Aug 2022 18:37
 Operator : SY/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.172	3144	3151	3153	rBV7	868	851	0.05%	0.007%
78	11.204	3159	3161	3162	rBV	769	362	0.02%	0.003%
79	11.249	3163	3175	3200	rBV	566491	887871	53.93%	7.167%
80	11.583	3276	3279	3280	rBV3	1215	655	0.04%	0.005%
81	11.622	3280	3291	3310	rVV	612875	983915	59.77%	7.943%
82	11.943	3389	3391	3395	rVB6	1058	692	0.04%	0.006%
83	12.477	3554	3557	3558	rBV	555	299	0.02%	0.002%
84	12.693	3621	3624	3625	rBV2	563	376	0.02%	0.003%
85	12.767	3644	3647	3649	rBV3	830	482	0.03%	0.004%
86	13.024	3724	3727	3730	rBV4	703	538	0.03%	0.004%
87	13.384	3838	3839	3843	rBV3	730	326	0.02%	0.003%
88	13.525	3881	3883	3886	rBV3	608	354	0.02%	0.003%
89	13.554	3890	3892	3894	rBV2	744	333	0.02%	0.003%
90	13.648	3918	3921	3923	rBV	631	456	0.03%	0.004%
91	13.853	3983	3985	3987	rBV3	632	383	0.02%	0.003%
92	13.898	3996	3999	4000	rBV2	1120	609	0.04%	0.005%
93	14.043	4040	4044	4046	rBV3	1003	644	0.04%	0.005%
94	14.400	4153	4155	4158	rBV2	727	459	0.03%	0.004%
95	14.439	4163	4167	4168	rBV2	618	423	0.03%	0.003%
96	14.471	4176	4177	4180	rBV2	517	284	0.02%	0.002%
97	14.509	4185	4189	4193	rBV3	1228	1172	0.07%	0.009%
98	14.750	4262	4264	4269	rBV4	670	450	0.03%	0.004%
99	14.850	4293	4295	4298	rBV3	990	445	0.03%	0.004%
100	15.252	4418	4420	4423	rBV4	939	670	0.04%	0.005%




Sum of corrected areas: 12387863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027233.D
Acq On : 05 Aug 2022 18:37
Operator : SY/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

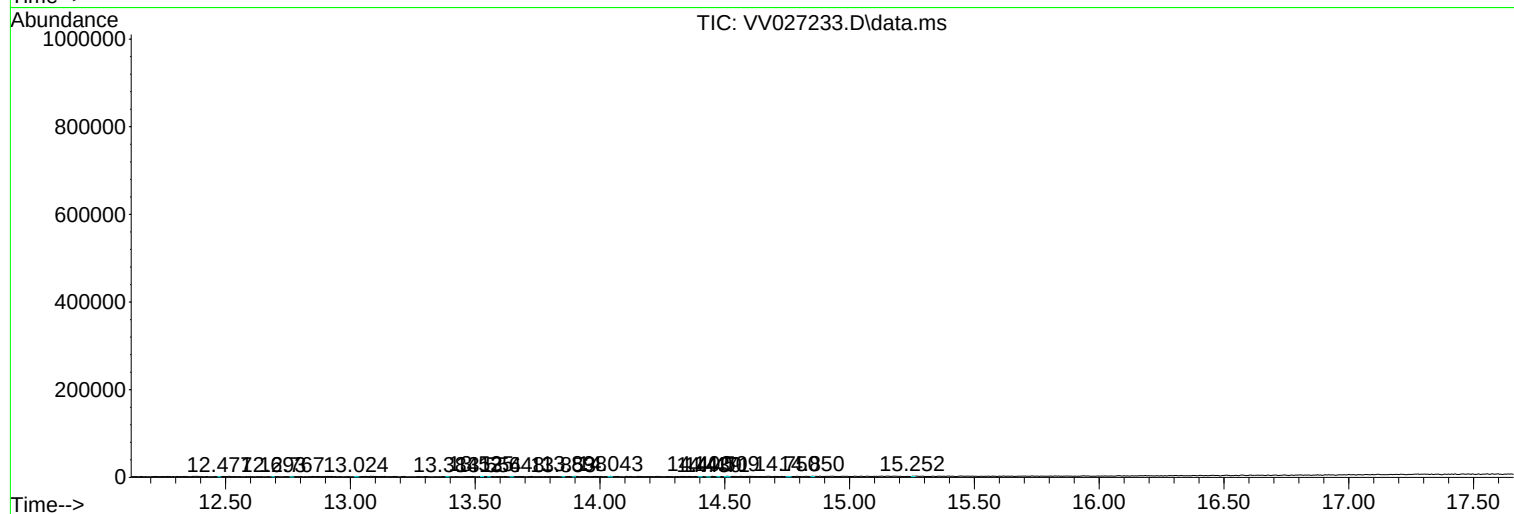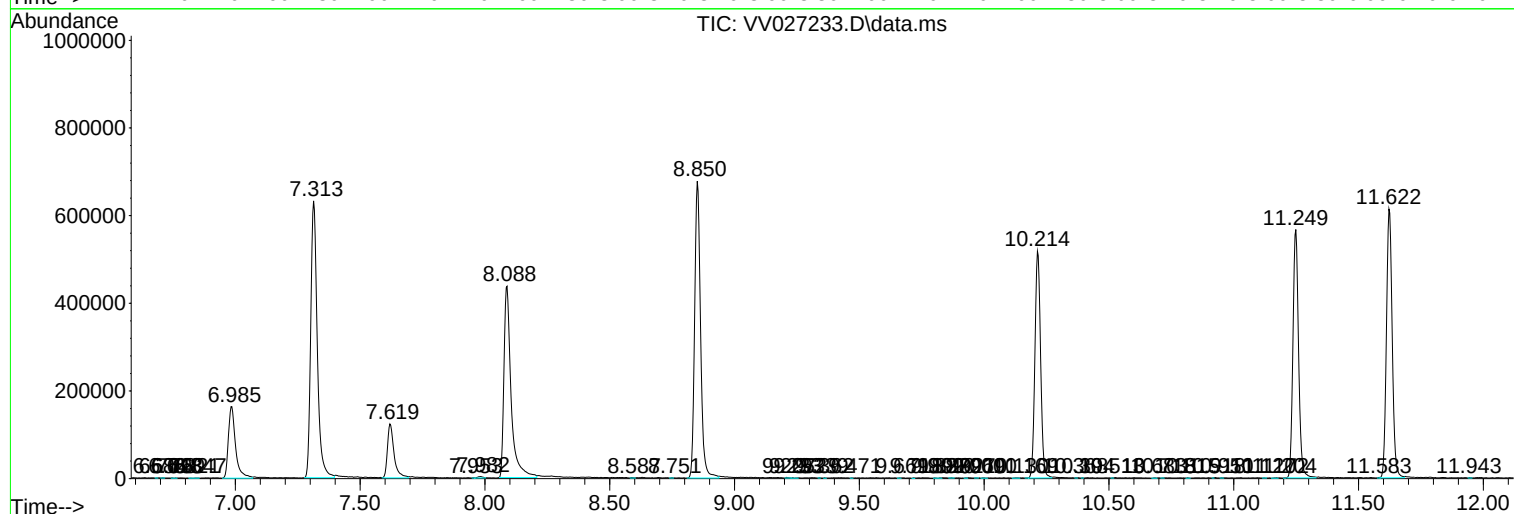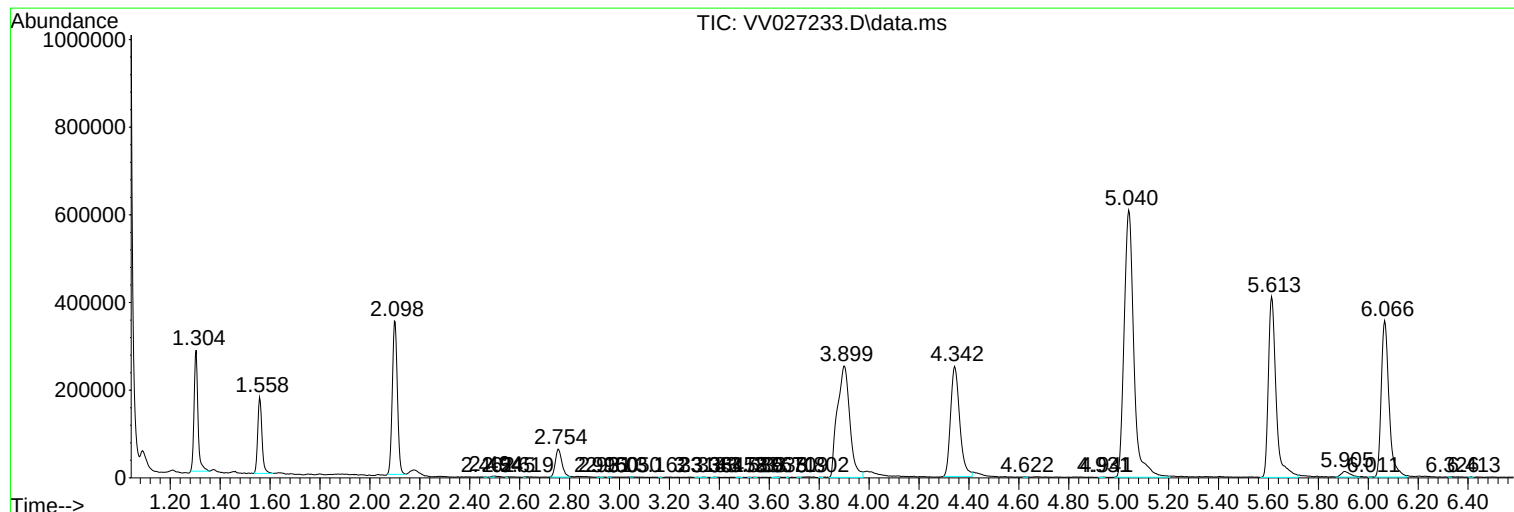

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027233.D
Acq On : 05 Aug 2022 18:37
Operator : SY/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027233.D
Acq On : 05 Aug 2022 18:37
Operator : SY/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc