

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027234.D
 Acq On : 05 Aug 2022 19:02
 Operator : SY/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV2	753341	846834	39.41%	5.955%
2	1.558	155	161	175	rVB	168528	195588	9.10%	1.375%
3	2.098	320	329	345	rBV	347345	492764	22.93%	3.465%
4	2.455	438	440	443	rBV3	823	398	0.02%	0.003%
5	2.500	448	454	461	rVV8	2222	3102	0.14%	0.022%
6	2.687	508	512	513	rBV2	751	520	0.02%	0.004%
7	2.754	521	533	552	rBV	124993	229337	10.67%	1.613%
8	3.015	612	614	618	rBV2	489	444	0.02%	0.003%
9	3.224	675	679	680	rBV	746	428	0.02%	0.003%
10	3.272	690	694	699	rBV4	943	784	0.04%	0.006%
11	3.339	711	715	716	rBV2	575	350	0.02%	0.002%
12	3.410	735	737	741	rVB3	612	374	0.02%	0.003%
13	3.478	753	758	759	rBV5	1206	988	0.05%	0.007%
14	3.561	782	784	787	rBV3	696	333	0.02%	0.002%
15	3.706	827	829	831	rBV	572	321	0.01%	0.002%
16	3.735	836	838	839	rBV	807	329	0.02%	0.002%
17	3.796	855	857	860	rVB3	905	556	0.03%	0.004%
18	3.815	860	863	869	rBV4	655	621	0.03%	0.004%
19	3.902	869	890	911	rBV2	781167	2149043	100.00%	15.112%
20	4.343	1012	1027	1057	rBV	245244	646889	30.10%	4.549%
21	4.841	1180	1182	1185	rBV4	635	339	0.02%	0.002%
22	4.902	1198	1201	1205	rVV3	1351	917	0.04%	0.006%
23	5.040	1227	1244	1294	rBV2	603805	1638046	76.22%	11.519%
24	5.439	1366	1368	1370	rVB3	1072	420	0.02%	0.003%
25	5.458	1370	1374	1375	rBV2	1110	706	0.03%	0.005%
26	5.545	1399	1401	1404	rVB3	681	357	0.02%	0.003%
27	5.613	1410	1422	1463	rVV	419706	900184	41.89%	6.330%
28	6.002	1541	1543	1545	rBV2	753	345	0.02%	0.002%
29	6.066	1550	1563	1592	rVV	353179	753632	35.07%	5.300%
30	6.313	1638	1640	1644	rBV4	704	434	0.02%	0.003%
31	6.355	1651	1653	1655	rBV3	690	292	0.01%	0.002%
32	6.429	1672	1676	1677	rBV4	799	524	0.02%	0.004%
33	6.439	1677	1679	1684	rVV6	568	513	0.02%	0.004%
34	6.551	1710	1714	1715	rBV3	635	334	0.02%	0.002%
35	6.577	1720	1722	1724	rBV3	655	381	0.02%	0.003%
36	6.616	1732	1734	1735	rBV2	726	353	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW080522\
 Data File : VW027234.D
 Acq On : 05 Aug 2022 19:02
 Operator : SY/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.651	1740	1745	1749	rBV5	982	959	0.04%	0.007%
38	6.693	1756	1758	1760	rVB	739	288	0.01%	0.002%
39	6.728	1765	1769	1770	rBV2	577	387	0.02%	0.003%
40	6.760	1777	1779	1783	rVB5	858	426	0.02%	0.003%
41	6.815	1794	1796	1798	rBV2	704	408	0.02%	0.003%
42	6.847	1804	1806	1808	rVB2	750	301	0.01%	0.002%
43	6.982	1838	1848	1869	rBV	160232	305937	14.24%	2.151%
44	7.313	1939	1951	1977	rBV	611951	1128137	52.49%	7.933%
45	7.619	2036	2046	2067	rBV	120079	220761	10.27%	1.552%
46	8.034	2173	2175	2177	rBV3	652	331	0.02%	0.002%
47	8.088	2181	2192	2231	rBV	445924	889537	41.39%	6.255%
48	8.850	2418	2429	2452	rBV	672541	1113056	51.79%	7.827%
49	9.339	2578	2581	2582	rBV3	721	358	0.02%	0.003%
50	9.432	2607	2610	2614	rBV5	825	534	0.02%	0.004%
51	9.555	2643	2648	2649	rBV3	1227	912	0.04%	0.006%
52	9.667	2681	2683	2687	rBV3	681	546	0.03%	0.004%
53	9.686	2687	2689	2694	rVB3	702	527	0.02%	0.004%
54	9.796	2720	2723	2725	rBV2	542	289	0.01%	0.002%
55	9.979	2779	2780	2784	rVB2	868	490	0.02%	0.003%
56	10.001	2784	2787	2790	rBV3	673	555	0.03%	0.004%
57	10.053	2801	2803	2805	rBV	774	439	0.02%	0.003%
58	10.214	2841	2853	2874	rVV	509372	805791	37.50%	5.666%
59	10.481	2934	2936	2939	rVV2	663	394	0.02%	0.003%
60	10.583	2962	2968	2970	rBV4	946	794	0.04%	0.006%
61	10.648	2986	2988	2992	rBV5	772	517	0.02%	0.004%
62	10.702	3000	3005	3007	rBV4	620	453	0.02%	0.003%
63	10.731	3012	3014	3017	rBV2	430	291	0.01%	0.002%
64	10.767	3021	3025	3028	rBV4	427	307	0.01%	0.002%
65	10.841	3044	3048	3050	rBV4	673	545	0.03%	0.004%
66	10.895	3062	3065	3071	rVB4	812	720	0.03%	0.005%
67	10.947	3078	3081	3084	rBV4	682	643	0.03%	0.005%
68	11.037	3105	3109	3110	rBV2	857	610	0.03%	0.004%
69	11.075	3117	3121	3125	rBV4	969	1026	0.05%	0.007%
70	11.165	3146	3149	3151	rBV2	522	314	0.01%	0.002%
71	11.194	3151	3158	3162	rVB8	794	1073	0.05%	0.008%
72	11.249	3162	3175	3194	rBV	576409	896262	41.71%	6.303%
73	11.622	3279	3291	3310	rBV	606914	963483	44.83%	6.775%
74	11.898	3373	3377	3379	rBV3	693	540	0.03%	0.004%
75	11.972	3398	3400	3403	rBV3	787	334	0.02%	0.002%
76	12.194	3465	3469	3473	rVB5	1045	797	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027234.D
 Acq On : 05 Aug 2022 19:02
 Operator : SY/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	12.217	3473	3476	3478	rBV4	888	460	0.02%	0.003%
78	12.313	3503	3506	3507	rBV2	719	342	0.02%	0.002%
79	12.361	3518	3521	3528	rBV5	746	838	0.04%	0.006%
80	12.519	3567	3570	3572	rBV4	1032	780	0.04%	0.005%
81	12.548	3577	3579	3580	rBV	945	456	0.02%	0.003%
82	12.603	3592	3596	3597	rBV	780	590	0.03%	0.004%
83	12.712	3625	3630	3632	rBV4	944	945	0.04%	0.007%
84	12.741	3637	3639	3644	rVB4	910	690	0.03%	0.005%
85	12.828	3665	3666	3669	rBV2	480	297	0.01%	0.002%
86	12.976	3711	3712	3715	rBV2	494	321	0.01%	0.002%
87	13.040	3729	3732	3734	rBV4	905	538	0.03%	0.004%
88	13.120	3755	3757	3760	rBV3	676	404	0.02%	0.003%
89	13.175	3772	3774	3778	rVB5	815	486	0.02%	0.003%
90	13.210	3782	3785	3789	rVV4	628	487	0.02%	0.003%
91	13.259	3799	3800	3803	rBV2	563	301	0.01%	0.002%
92	13.429	3851	3853	3856	rBV	681	373	0.02%	0.003%
93	13.812	3970	3972	3976	rVB2	795	422	0.02%	0.003%
94	13.889	3993	3996	4002	rVV5	1186	1084	0.05%	0.008%
95	14.014	4033	4035	4037	rBV3	790	336	0.02%	0.002%
96	14.194	4087	4091	4094	rBV3	834	767	0.04%	0.005%
97	14.352	4138	4140	4141	rBV2	786	323	0.02%	0.002%
98	14.387	4149	4151	4154	rVB3	718	372	0.02%	0.003%
99	14.448	4168	4170	4174	rBV3	848	644	0.03%	0.005%
100	15.159	4389	4391	4392	rBV	812	302	0.01%	0.002%




Sum of corrected areas: 14220410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027234.D
Acq On : 05 Aug 2022 19:02
Operator : SY/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

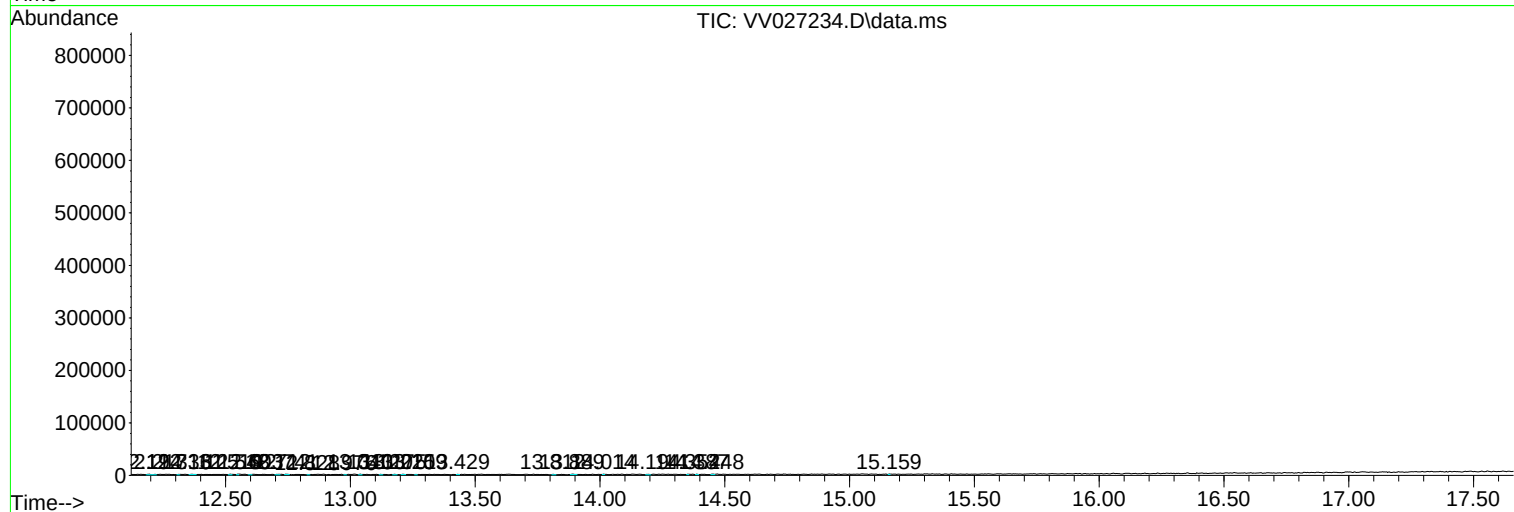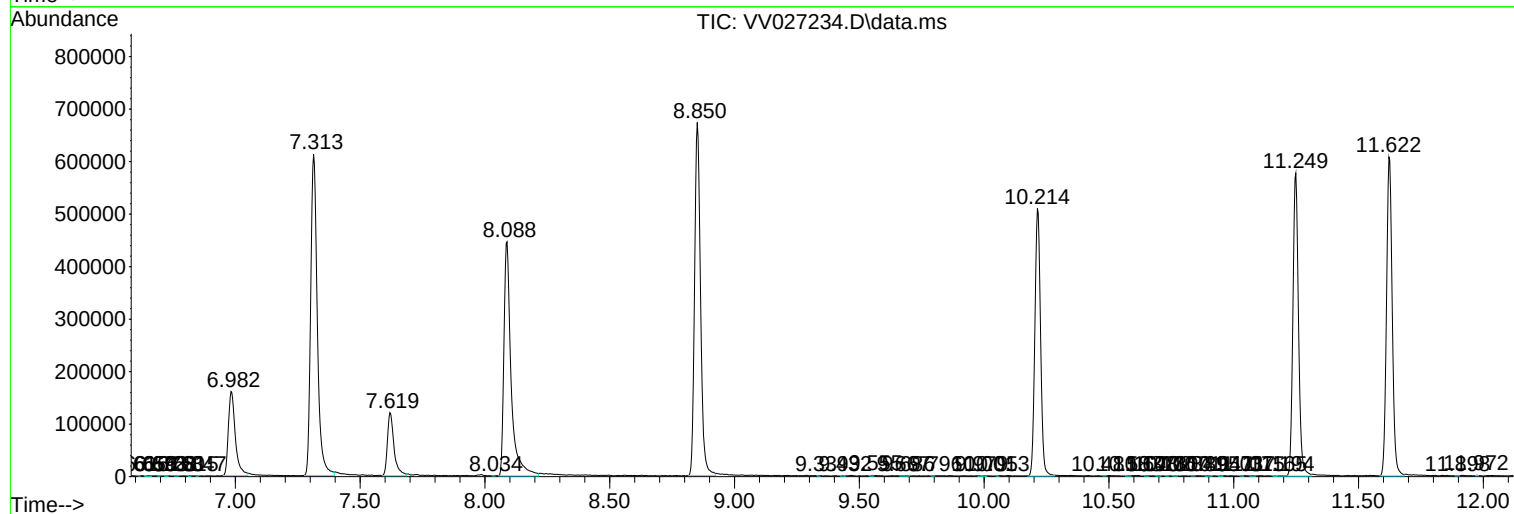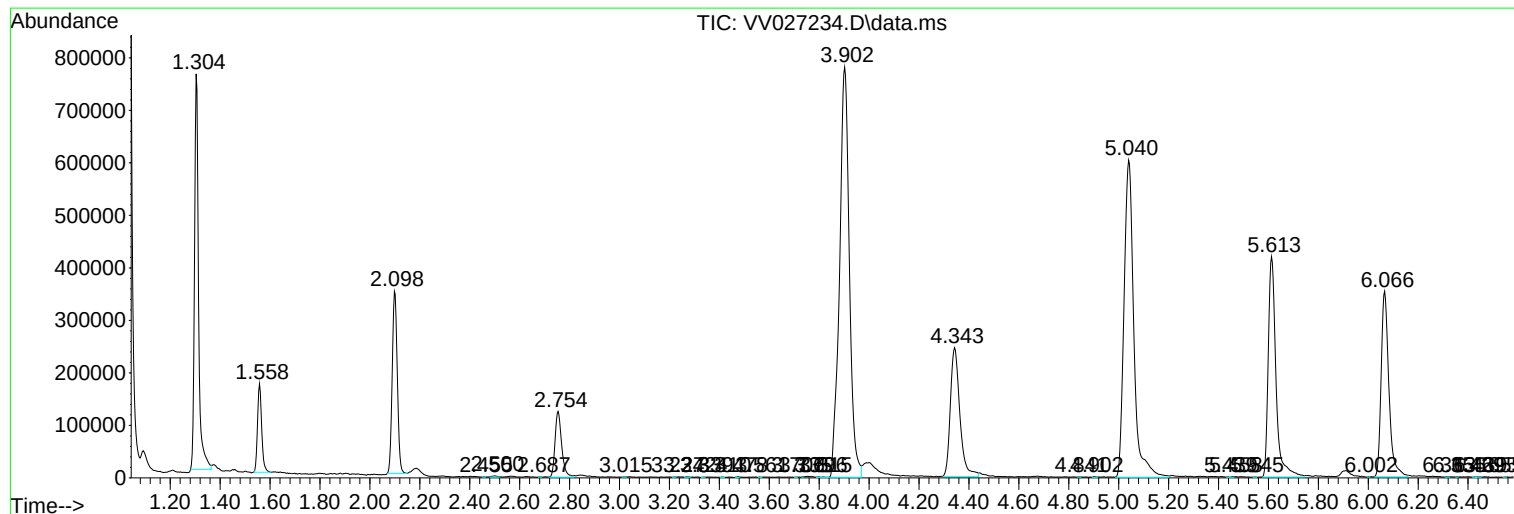

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027234.D
Acq On : 05 Aug 2022 19:02
Operator : SY/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027234.D
Acq On : 05 Aug 2022 19:02
Operator : SY/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc