

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027236.D
 Acq On : 05 Aug 2022 19:52
 Operator : SY/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rBV2	1066323	1206719	4.77%	2.536%
2	1.558	155	161	176	rVB	163891	194906	0.77%	0.410%
3	2.101	320	330	345	rBV	347535	496791	1.97%	1.044%
4	2.507	448	456	463	rBV9	2363	3981	0.02%	0.008%
5	2.600	483	485	488	rVB2	780	310	0.00%	0.001%
6	2.754	522	533	552	rBV	121359	215672	0.85%	0.453%
7	2.908	578	581	583	rBV4	824	403	0.00%	0.001%
8	2.966	595	599	602	rBV3	765	766	0.00%	0.002%
9	2.992	605	607	609	rBV3	590	294	0.00%	0.001%
10	3.056	625	627	629	rBV2	507	245	0.00%	0.001%
11	3.082	632	635	638	rVB3	784	449	0.00%	0.001%
12	3.098	638	640	641	rBV2	557	226	0.00%	0.000%
13	3.143	649	654	655	rBV3	624	480	0.00%	0.001%
14	3.172	660	663	666	rBV2	574	413	0.00%	0.001%
15	3.211	673	675	678	rBV	646	353	0.00%	0.001%
16	3.233	680	682	687	rVB4	719	502	0.00%	0.001%
17	3.310	704	706	708	rBV2	350	174	0.00%	0.000%
18	3.323	708	710	713	rVB2	727	382	0.00%	0.001%
19	3.339	713	715	717	rBV	274	139	0.00%	0.000%
20	3.355	717	720	722	rBV2	725	430	0.00%	0.001%
21	3.388	729	730	734	rVB3	549	213	0.00%	0.000%
22	3.445	746	748	751	rVB2	316	187	0.00%	0.000%
23	3.468	751	755	757	rVB3	584	383	0.00%	0.001%
24	3.487	757	761	763	rBV2	453	362	0.00%	0.001%
25	3.503	763	766	769	rVB3	380	235	0.00%	0.000%
26	3.539	775	777	779	rBV	351	201	0.00%	0.000%
27	3.568	781	786	787	rBV3	324	270	0.00%	0.001%
28	3.593	792	794	798	rBV3	332	285	0.00%	0.001%
29	3.622	802	803	807	rVB3	644	267	0.00%	0.001%
30	3.642	807	809	811	rVB2	398	194	0.00%	0.000%
31	3.670	811	818	819	rBV2	770	802	0.00%	0.002%
32	3.696	824	826	829	rBV3	503	283	0.00%	0.001%
33	3.732	835	837	839	rBV2	448	175	0.00%	0.000%
34	3.764	842	847	849	rBV3	713	568	0.00%	0.001%
35	3.812	859	862	865	rBV2	634	405	0.00%	0.001%
36	3.902	871	890	909	rBV	3351306	8013785	31.71%	16.844%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW080522\
 Data File : VW027236.D
 Acq On : 05 Aug 2022 19:52
 Operator : SY/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	4.342	1014	1027	1049	rBV	246172	618437	2.45%	1.300%
38	4.760	1155	1157	1158	rBV2	641	300	0.00%	0.001%
39	4.815	1172	1174	1178	rVB2	767	426	0.00%	0.001%
40	4.838	1178	1181	1183	rBV4	747	541	0.00%	0.001%
41	4.860	1186	1188	1190	rVV2	553	215	0.00%	0.000%
42	4.902	1196	1201	1203	rBV4	1100	994	0.00%	0.002%
43	5.040	1228	1244	1289	rBV2	594661	1599329	6.33%	3.362%
44	5.394	1351	1354	1357	rBV3	1522	1000	0.00%	0.002%
45	5.613	1410	1422	1464	rBV	401612	873764	3.46%	1.837%
46	5.908	1498	1514	1551	rBV	12753487	25274279	100.00%	53.123%
47	6.066	1554	1563	1595	rVB	360071	774018	3.06%	1.627%
48	6.805	1789	1793	1795	rBV3	1196	938	0.00%	0.002%
49	6.838	1800	1803	1804	rBV3	795	381	0.00%	0.001%
50	6.905	1820	1824	1825	rBV3	598	410	0.00%	0.001%
51	6.982	1838	1848	1875	rBV	159816	313172	1.24%	0.658%
52	7.313	1939	1951	1974	rBV	622346	1121988	4.44%	2.358%
53	7.619	2037	2046	2070	rBV2	117199	214371	0.85%	0.451%
54	7.973	2142	2156	2182	rBV	1180857	2030327	8.03%	4.267%
55	8.088	2182	2192	2231	rVV	447208	859193	3.40%	1.806%
56	8.757	2398	2400	2405	rVB4	938	588	0.00%	0.001%
57	8.850	2417	2429	2453	rBV	643502	1082774	4.28%	2.276%
58	9.281	2560	2563	2564	rBV2	872	451	0.00%	0.001%
59	9.403	2598	2601	2606	rBV4	413	388	0.00%	0.001%
60	9.545	2643	2645	2646	rBV2	355	135	0.00%	0.000%
61	9.571	2651	2653	2656	rBV3	394	221	0.00%	0.000%
62	9.625	2668	2670	2673	rVB3	636	356	0.00%	0.001%
63	9.638	2673	2674	2676	rBV	687	223	0.00%	0.000%
64	9.776	2714	2717	2720	rBV3	602	364	0.00%	0.001%
65	9.796	2721	2723	2725	rBV2	772	404	0.00%	0.001%
66	9.886	2749	2751	2755	rVB3	596	385	0.00%	0.001%
67	9.908	2755	2758	2759	rBV	423	208	0.00%	0.000%
68	9.940	2765	2768	2769	rBV2	932	389	0.00%	0.001%
69	9.960	2773	2774	2776	rVV	482	160	0.00%	0.000%
70	10.066	2805	2807	2809	rBV	335	182	0.00%	0.000%
71	10.082	2809	2812	2815	rBV3	476	398	0.00%	0.001%
72	10.214	2839	2853	2879	rBV	510478	804796	3.18%	1.692%
73	10.554	2957	2959	2960	rBV2	382	127	0.00%	0.000%
74	10.709	3005	3007	3008	rBV2	483	173	0.00%	0.000%
75	10.738	3014	3016	3017	rBV2	451	174	0.00%	0.000%
76	10.837	3045	3047	3048	rBV	499	207	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027236.D
 Acq On : 05 Aug 2022 19:52
 Operator : SY/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.850	3049	3051	3055	rVV5	922	667	0.00%	0.001%
78	10.921	3071	3073	3074	rBV	482	179	0.00%	0.000%
79	11.104	3127	3130	3132	rBV3	532	374	0.00%	0.001%
80	11.169	3148	3150	3152	rBV2	643	373	0.00%	0.001%
81	11.198	3158	3159	3161	rBV	393	183	0.00%	0.000%
82	11.249	3163	3175	3192	rBV	551499	871891	3.45%	1.833%
83	11.622	3279	3291	3314	rBV	620786	977137	3.87%	2.054%
84	11.882	3368	3372	3375	rBV3	1119	960	0.00%	0.002%
85	12.143	3451	3453	3457	rVB3	802	403	0.00%	0.001%
86	12.696	3623	3625	3628	rBV4	759	407	0.00%	0.001%
87	12.831	3665	3667	3669	rBV2	483	249	0.00%	0.001%
88	12.850	3671	3673	3675	rBV2	755	428	0.00%	0.001%
89	13.040	3731	3732	3733	rBV2	407	136	0.00%	0.000%
90	13.246	3794	3796	3797	rBV	458	167	0.00%	0.000%
91	13.416	3845	3849	3851	rBV2	462	352	0.00%	0.001%
92	13.471	3864	3866	3868	rBV3	667	322	0.00%	0.001%
93	13.593	3903	3904	3905	rBV	455	125	0.00%	0.000%
94	13.603	3905	3907	3911	rVV4	732	547	0.00%	0.001%
95	13.644	3918	3920	3925	rBV4	768	640	0.00%	0.001%
96	13.879	3991	3993	3995	rBV3	595	207	0.00%	0.000%
97	13.988	4026	4027	4028	rBV	722	240	0.00%	0.001%
98	14.136	4071	4073	4075	rBV3	774	471	0.00%	0.001%
99	14.345	4134	4138	4141	rBV4	1041	1103	0.00%	0.002%
100	14.455	4170	4172	4173	rBV2	656	167	0.00%	0.000%




Sum of corrected areas: 47577164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027236.D
Acq On : 05 Aug 2022 19:52
Operator : SY/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

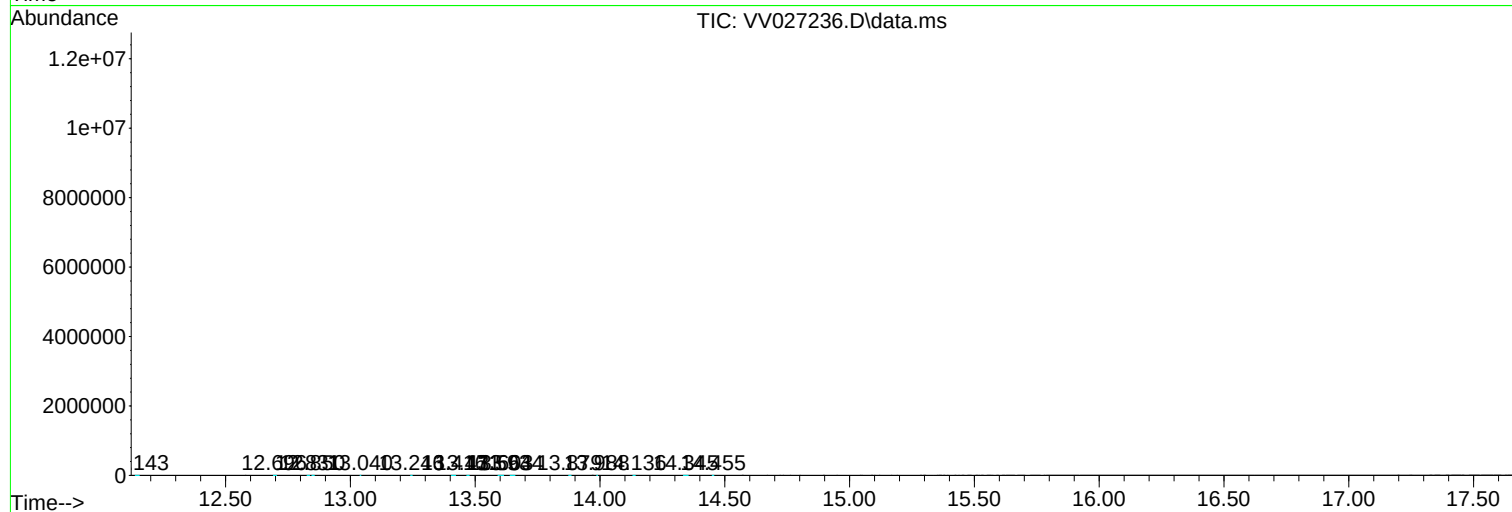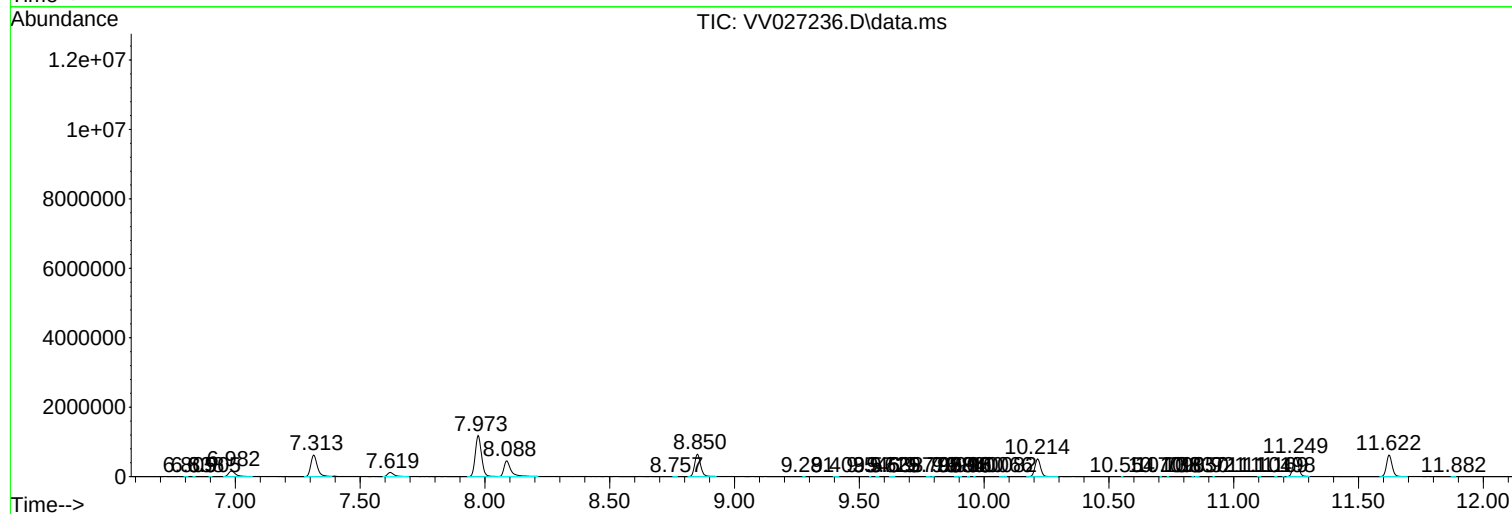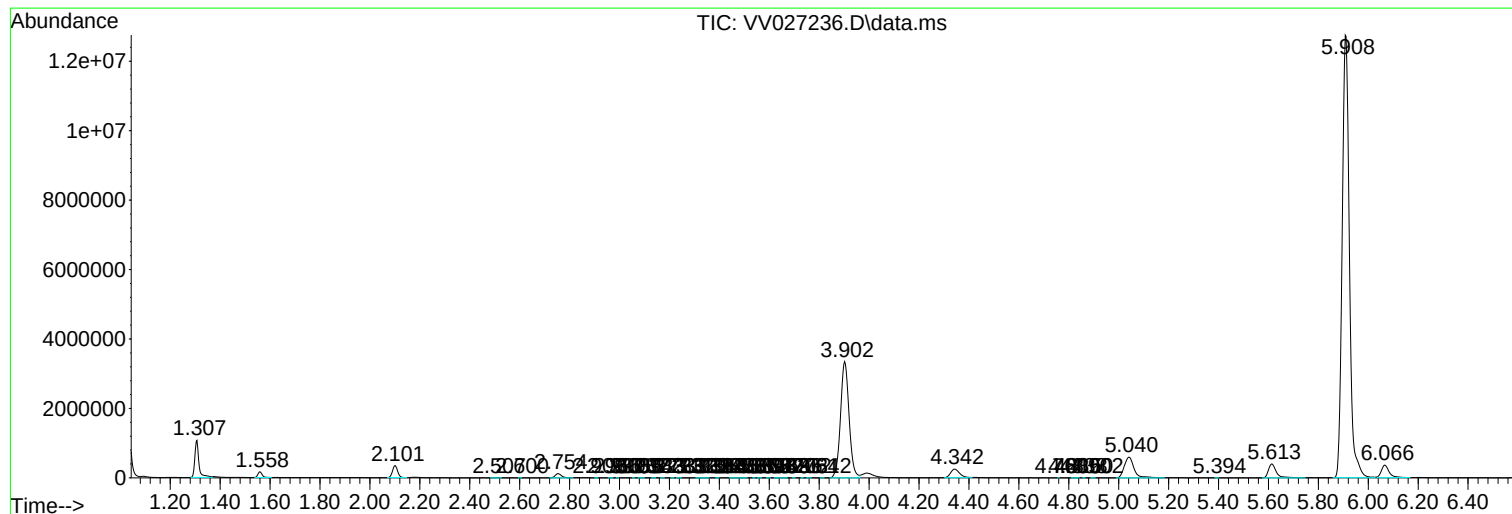

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027236.D
Acq On : 05 Aug 2022 19:52
Operator : SY/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
Data File : VV027236.D
Acq On : 05 Aug 2022 19:52
Operator : SY/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc