


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080522\
 Data File : VV027216.D
 Acq On : 05 Aug 2022 08:49
 Operator : SY/MD
 Sample : BFB306
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB306

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 06 03:57:43 2022

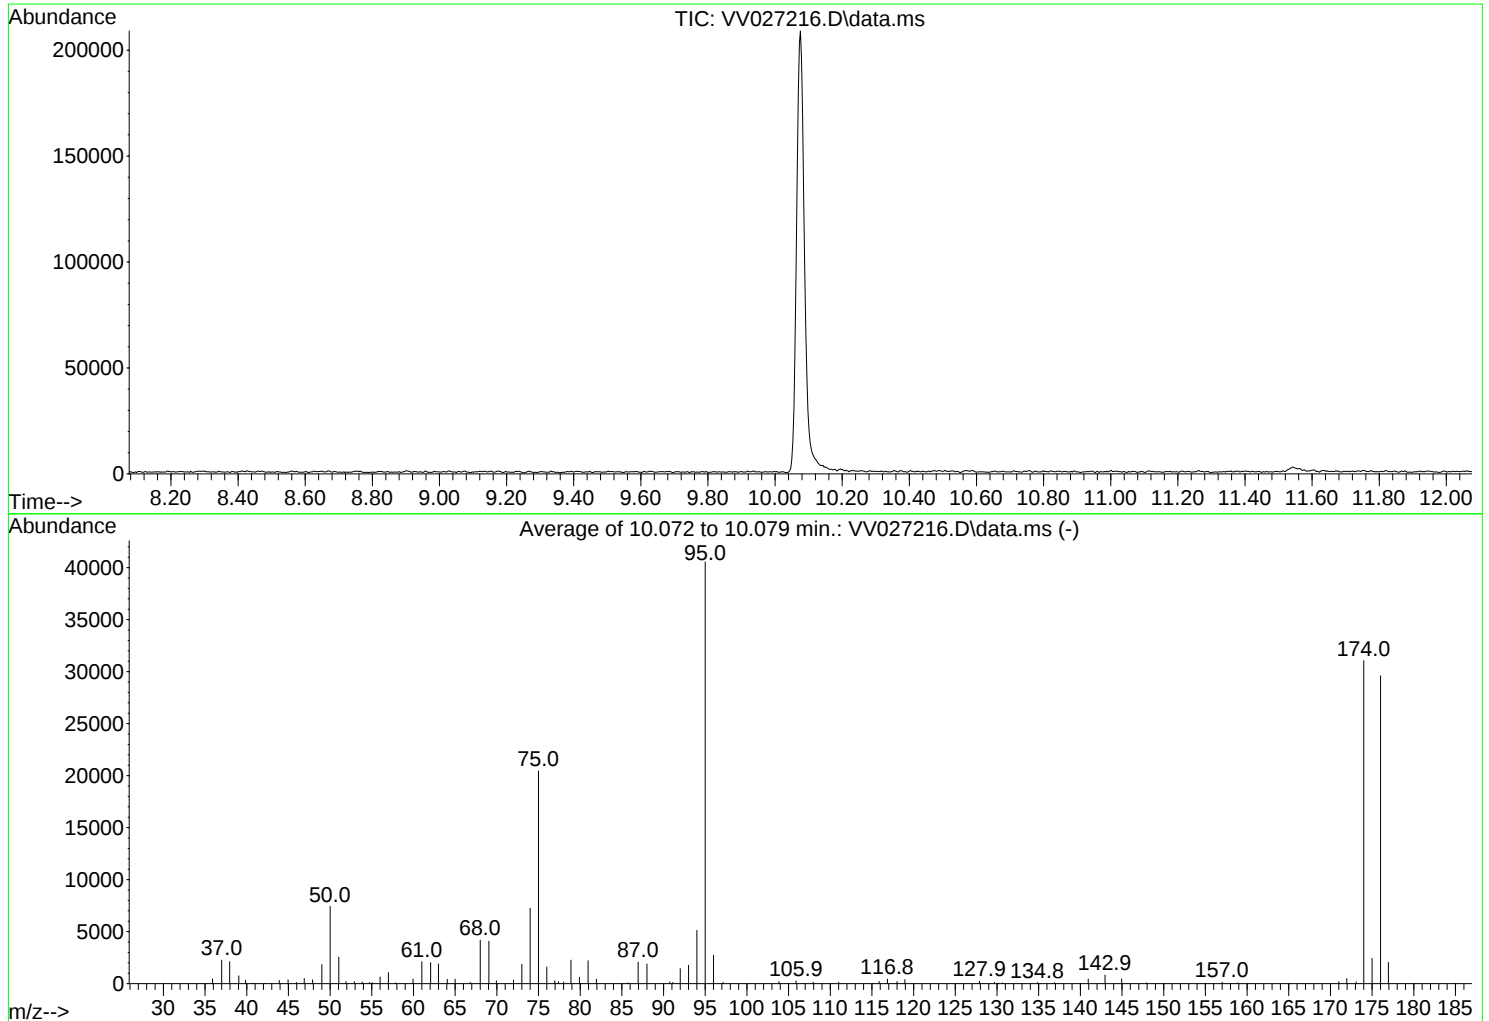

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	7426	PASS
75	95	30	80	50.4	20453	PASS
95	95	100	100	100.0	40560	PASS
96	95	5	9	6.7	2719	PASS
173	174	0.00	2	0.6	173	PASS
174	95	50	120	76.6	31053	PASS
175	174	5	9	7.8	2427	PASS
176	174	95	105	95.4	29611	PASS
177	176	5	10	6.9	2049	PASS

m/z	Abundance
40.10	234.0
43.10	104.0
43.90	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
35.90	531.0
37.00	2319.0
38.00	2021.0
39.10	842.0
39.90	292.0
44.00	616.0
44.90	355.0
45.90	119.0
46.90	583.0
47.90	350.0
49.00	1866.0
50.00	7914.0
51.00	2594.0
51.90	183.0
52.90	185.0
53.80	136.0
55.10	169.0
56.00	643.0
57.00	1075.0
60.00	430.0
61.00	2298.0
62.10	2047.0
63.00	1925.0
64.10	441.0
65.00	365.0
66.80	108.0
68.00	4362.0
69.00	4305.0
70.00	271.0
72.00	388.0
73.00	1889.0
74.00	7410.0
75.00	20768.0
76.00	1773.0
77.00	261.0
77.40	205.0
78.00	145.0
78.90	2354.0
79.90	627.0
81.00	2366.0
82.00	408.0
86.90	2099.0
88.00	1901.0
90.80	203.0
92.00	1371.0
93.00	1774.0
94.00	5180.0
95.00	41272.0
96.00	2724.0
97.20	136.0
103.90	190.0
105.00	111.0
105.90	226.0
106.70	109.0
108.00	111.0
111.00	113.0
115.90	258.0
116.90	391.0
118.00	184.0
118.90	386.0
127.90	240.0
129.70	120.0
130.20	119.0
134.90	110.0
140.90	447.0
142.90	835.0
144.90	446.0
157.00	101.0
171.00	198.0
172.00	460.0
174.00	30416.0
175.00	2343.0
176.00	28968.0
177.00	2085.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
35.90	485.0
37.00	2337.0
38.00	2158.0
39.10	752.0
39.80	333.0
44.00	611.0
45.00	390.0
46.00	130.0
46.90	503.0
47.90	384.0
49.00	1877.0
50.00	7689.0
51.10	2647.0
51.90	219.0
52.90	189.0
53.90	173.0
54.70	152.0
55.00	141.0
56.00	664.0
57.00	1072.0
57.90	106.0
60.00	441.0
61.00	2146.0
62.10	2028.0
63.00	1977.0
64.00	433.0
65.00	413.0
66.80	122.0
68.00	4316.0
69.00	4142.0
69.90	271.0
72.00	359.0
73.00	1890.0
74.00	7440.0
75.00	21032.0
76.00	1600.0
76.90	279.0
77.40	216.0
78.00	170.0
78.90	2324.0
79.90	673.0
80.90	2215.0
81.90	430.0
85.70	110.0
86.90	2128.0
88.00	1926.0
90.70	159.0
91.10	165.0
92.00	1499.0
93.00	1788.0
94.00	5337.0
95.00	41896.0
96.00	2814.0
97.20	129.0
103.80	214.0
105.70	186.0
106.00	200.0
108.00	131.0
111.00	148.0
115.20	117.0
115.80	204.0
116.80	449.0
118.00	204.0
118.90	384.0
127.90	239.0
129.70	119.0
130.60	108.0
134.80	120.0
136.90	121.0
140.90	458.0
143.00	879.0
145.00	481.0
147.90	114.0
157.00	147.0
158.90	104.0
171.00	190.0
172.00	487.0
174.00	32200.0
175.00	2497.0
176.00	30576.0
176.90	2068.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
35.90	389.0
37.00	2133.0
37.90	2128.0
39.00	695.0
39.80	368.0
40.70	135.0
42.20	107.0
42.90	120.0
43.90	626.0
45.00	373.0
46.00	117.0
46.90	384.0
47.90	376.0
49.00	1743.0
50.00	6674.0
51.10	2430.0
51.90	223.0
52.90	172.0
53.90	139.0
54.70	172.0
56.00	612.0
57.00	1032.0
57.80	105.0
59.90	494.0
61.00	1896.0
62.00	1963.0
63.00	1791.0
64.00	385.0
65.00	499.0
66.80	120.0
68.00	3892.0
69.10	3773.0
69.90	290.0
72.00	261.0
73.00	1814.0
74.00	6883.0
75.00	19560.0
76.00	1414.0
76.90	305.0
77.40	152.0
78.00	168.0
78.90	2123.0
79.90	566.0
80.90	2037.0
81.90	434.0
85.70	115.0
86.00	113.0
87.00	1971.0
88.00	1857.0
90.70	132.0
91.10	143.0
92.00	1471.0
93.00	1747.0
94.00	4874.0
95.00	38512.0
96.00	2620.0
97.10	101.0
103.80	219.0
106.00	188.0
107.90	169.0
111.00	146.0
115.80	175.0
116.80	456.0
118.00	207.0
119.00	363.0
127.90	193.0
129.70	120.0
130.70	107.0
134.80	115.0
136.90	143.0
141.00	444.0
143.00	799.0
145.00	449.0
148.00	112.0
157.00	129.0
158.80	101.0
171.00	171.0
171.90	511.0
173.10	518.0
174.00	30544.0
175.00	2440.0
176.00	29288.0
176.90	1994.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306